

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101323\
 Data File : VV032428.D
 Acq On : 13 Oct 2023 14:49
 Operator : SY/MD
 Sample : VV1013WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 16 02:53:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101323.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 16 02:50:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	7075	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.800	117	6719	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	3533	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	5781	0.499	ug/L	0.00
4) 1,2-Dichloroethane-d4	4.946	65	3576	0.487	ug/L	0.00
7) 1,2-Dichloropropane-d6	5.996	67	4538	0.492	ug/L	0.00
8) Toluene-d8	7.254	98	10352	0.472	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3039	0.479	ug/L	0.00
Target Compounds						
						Qvalue
6) Trichloroethene	5.853	95	155	0.022	ug/L	89
13) 1,2-Dibromo-3-chloropr...	12.357	75	8	0.011	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101323\
Data File : VV032428.D
Acq On : 13 Oct 2023 14:49
Operator : SY/MD
Sample : VV1013WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 16 02:53:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101323.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 16 02:50:34 2023
Response via : Initial Calibration

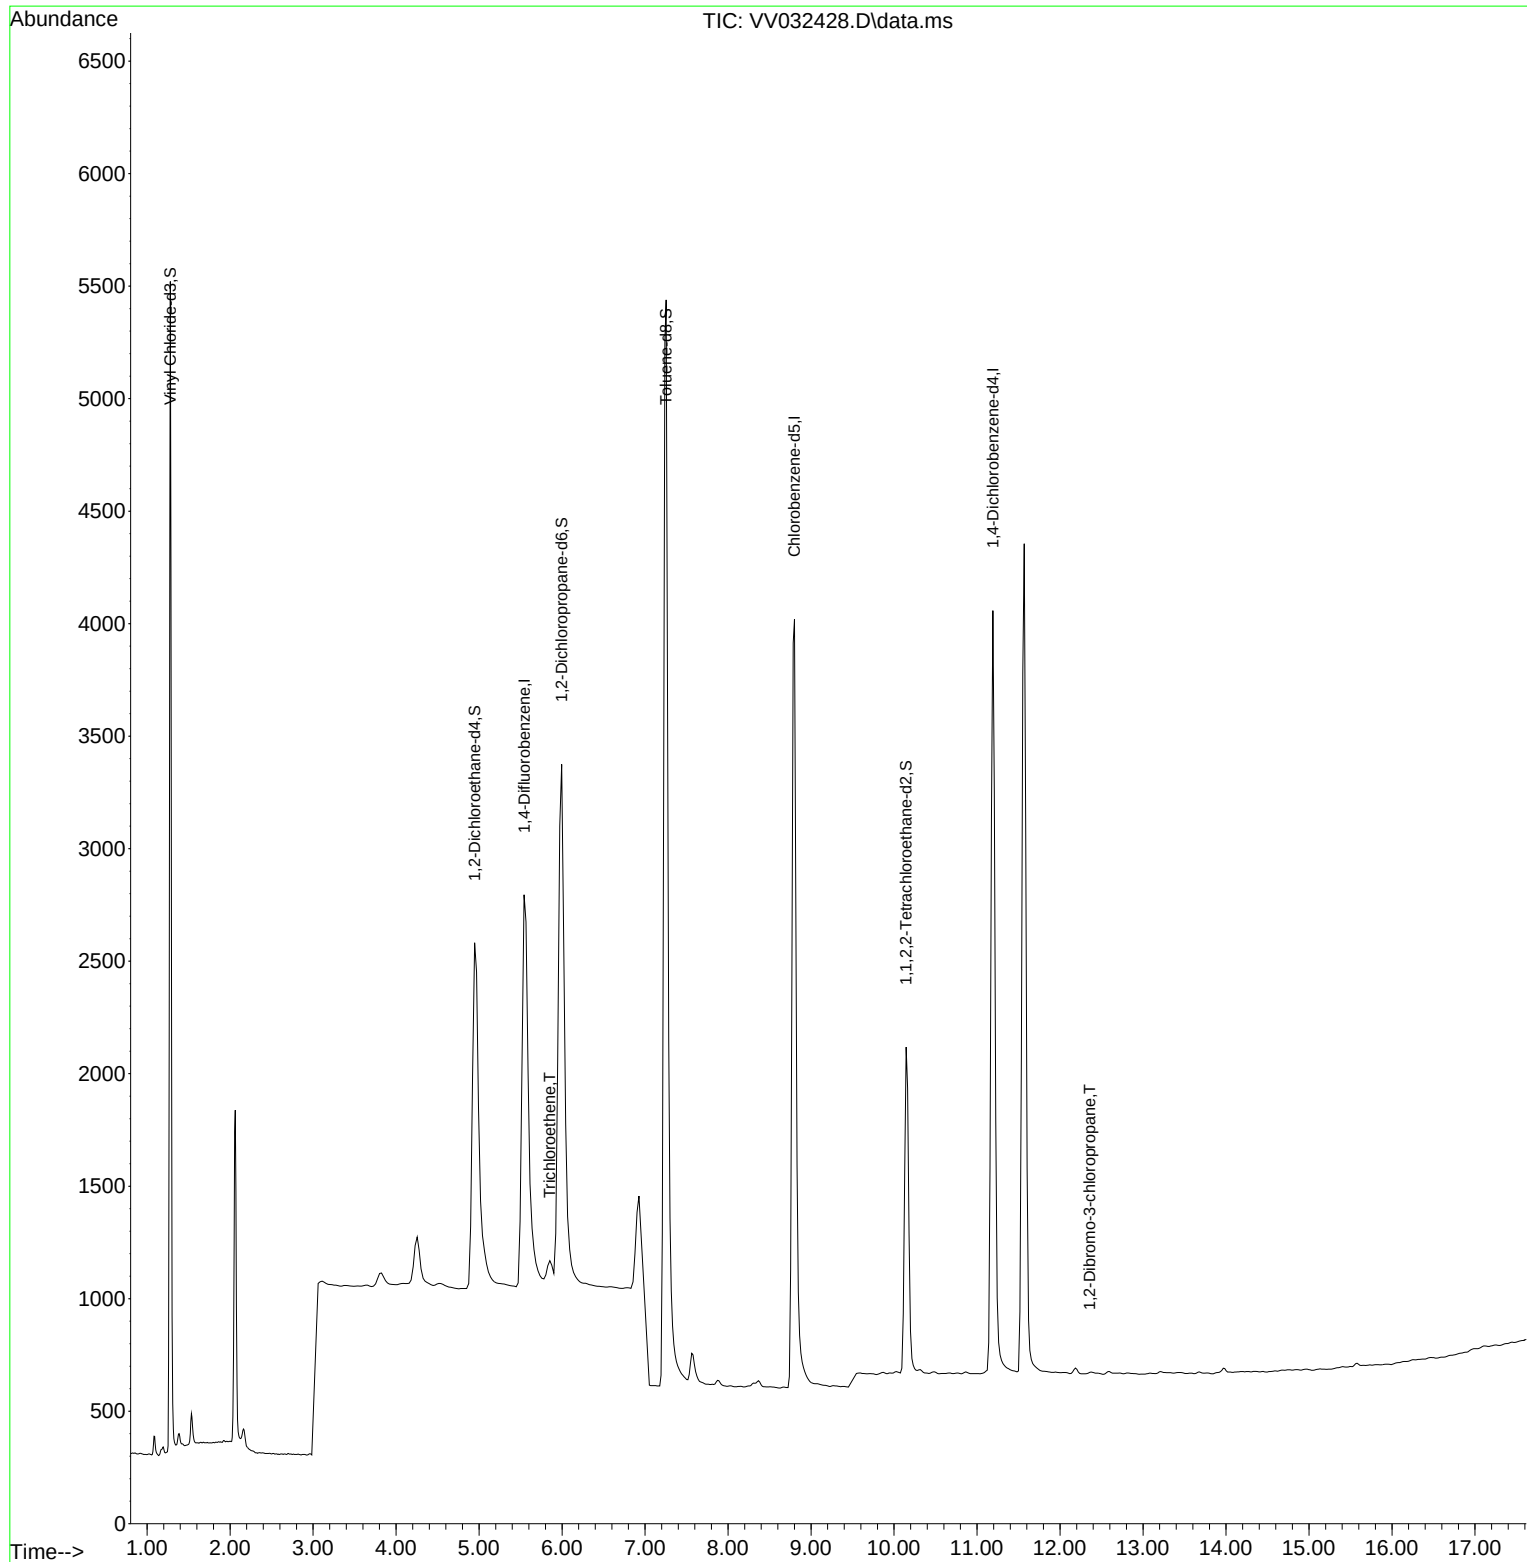

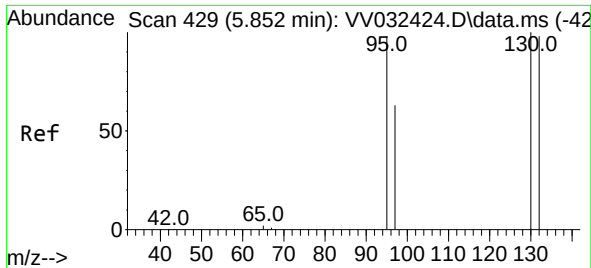




#6
 Trichloroethene
 Concen: 0.022 ug/L
 RT: 5.853 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VV032428.D
 Acq: 13 Oct 2023 14:49

Instrument :
 MSVOA_V
 ClientSampleId :

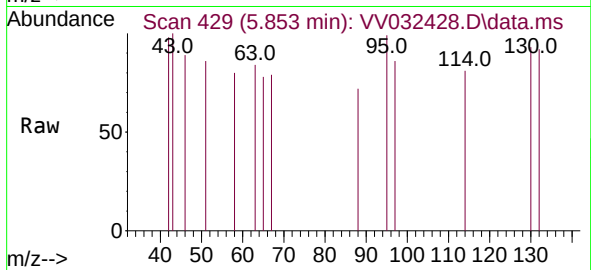

Tgt Ion: 95 Resp: 155

Ion	Ratio	Lower	Upper
95	100		
97	87.4	47.3	87.9
132	92.6	69.2	128.6
130	93.7	70.9	131.7

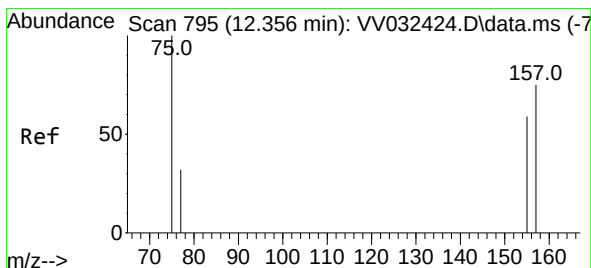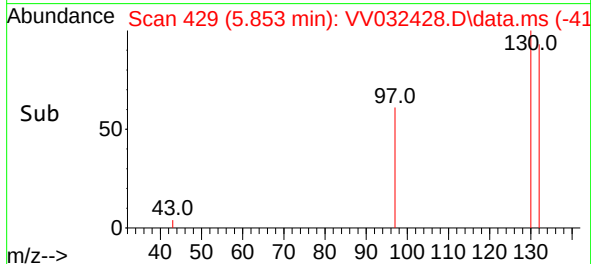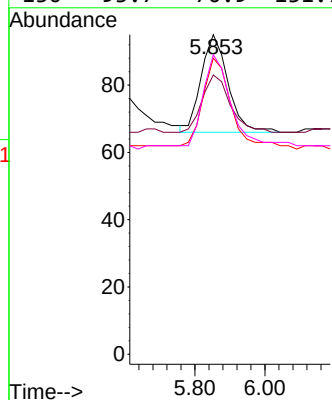

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.011 ug/L
 RT: 12.357 min Scan# 795
 Delta R.T. 0.000 min
 Lab File: VV032428.D
 Acq: 13 Oct 2023 14:49

Tgt Ion: 75 Resp: 8

Ion	Ratio	Lower	Upper
75	100		
157	77.9	61.0	91.6
155	79.2	54.2	81.4

