




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101323\
 Data File : VV032423.D
 Acq On : 13 Oct 2023 11:58
 Operator : SY/MD
 Sample : VSTD0.140
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1240

Manual IntegrationsAPPROVED

Quant Time: Oct 16 02:45:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101323.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 16 02:44:39 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/16/2023
 Supervised By :Semsettin Yesilyurt 10/16/2023

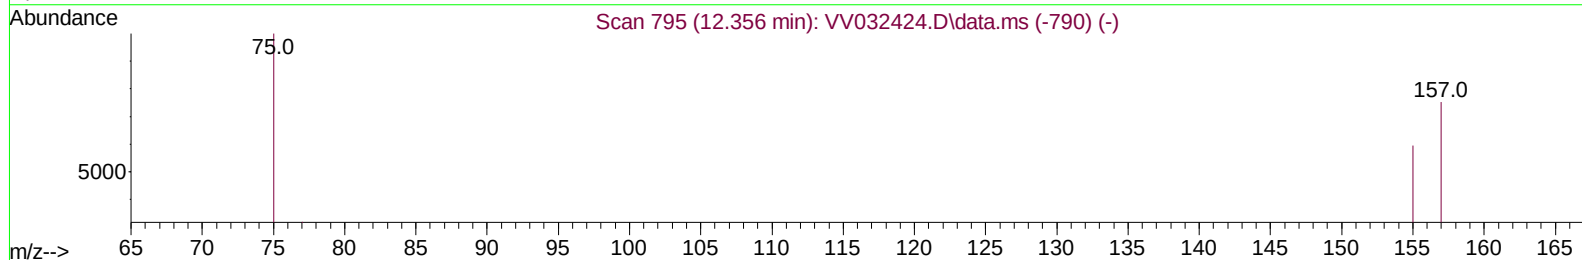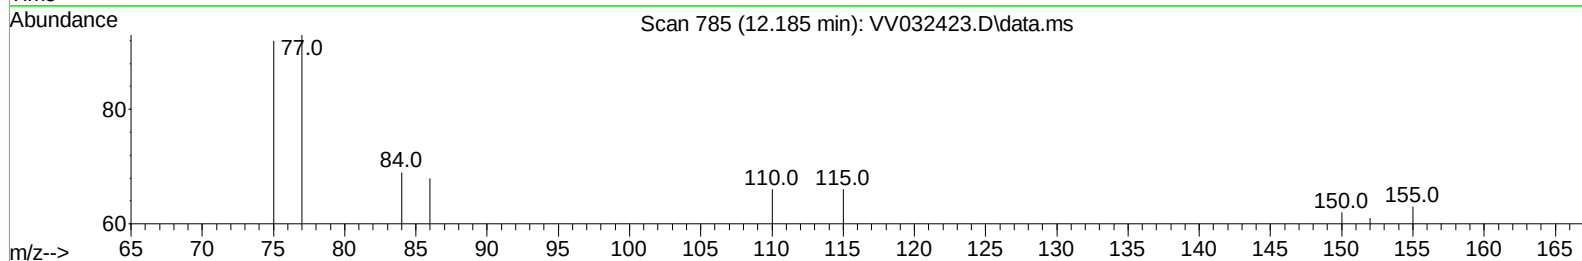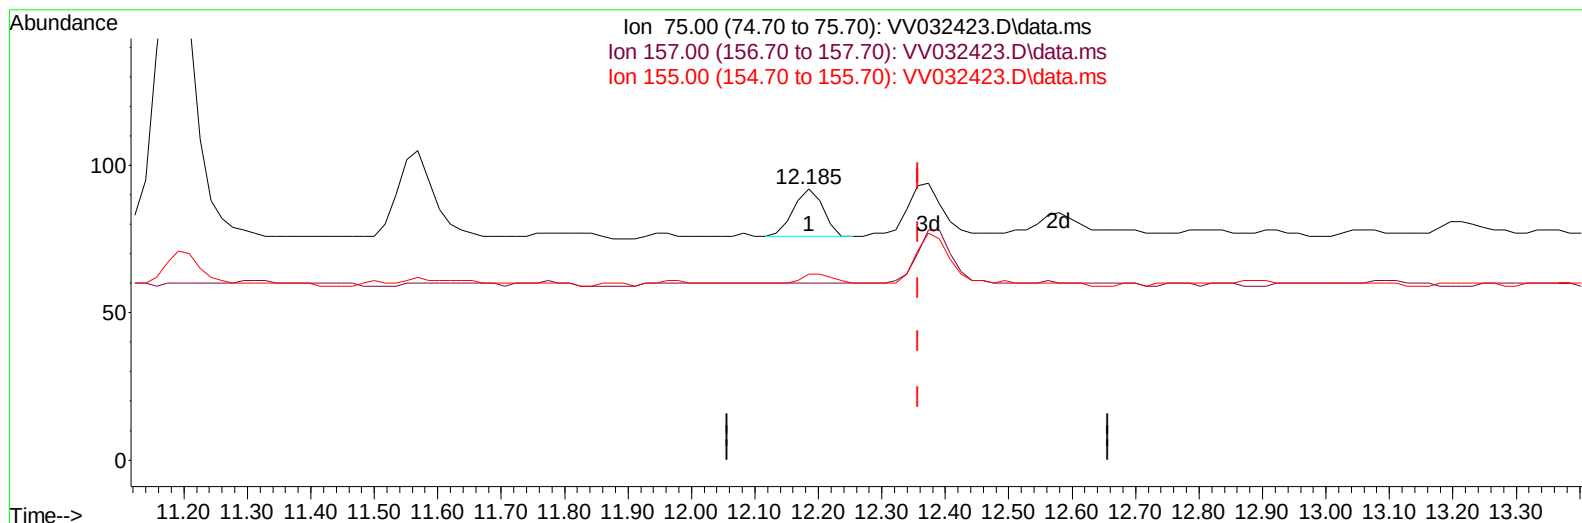

TIC: VV032423.D\data.ms

(13) 1,2-Dibromo-3-chloropropane (T)

12.185min (-0.171) 0.07 ug/L

response 51

Ion	Exp%	Act%
75.00	100.00	100.00
157.00	76.30	65.22
155.00	67.80	68.48
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101323\
 Data File : VV032423.D
 Acq On : 13 Oct 2023 11:58
 Operator : SY/MD
 Sample : VSTD0.140
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1240

Manual IntegrationsAPPROVED

Quant Time: Oct 16 02:45:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101323.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 16 02:44:39 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/16/2023
 Supervised By :Semsettin Yesilyurt 10/16/2023

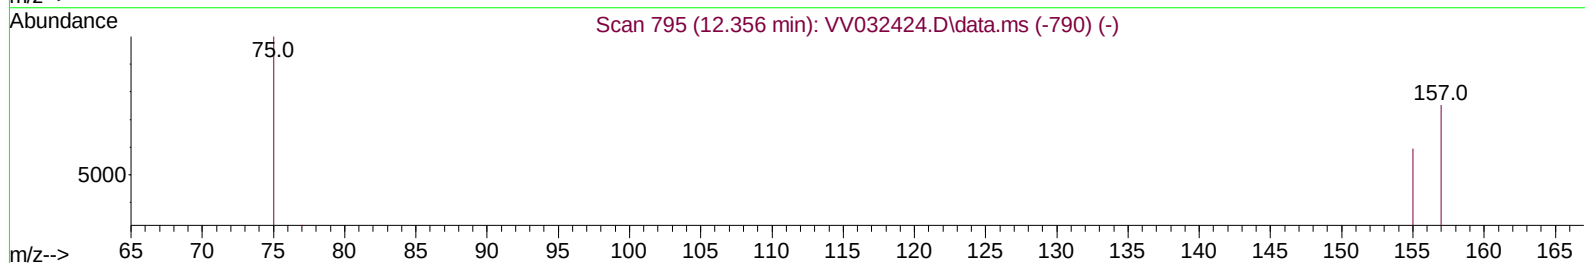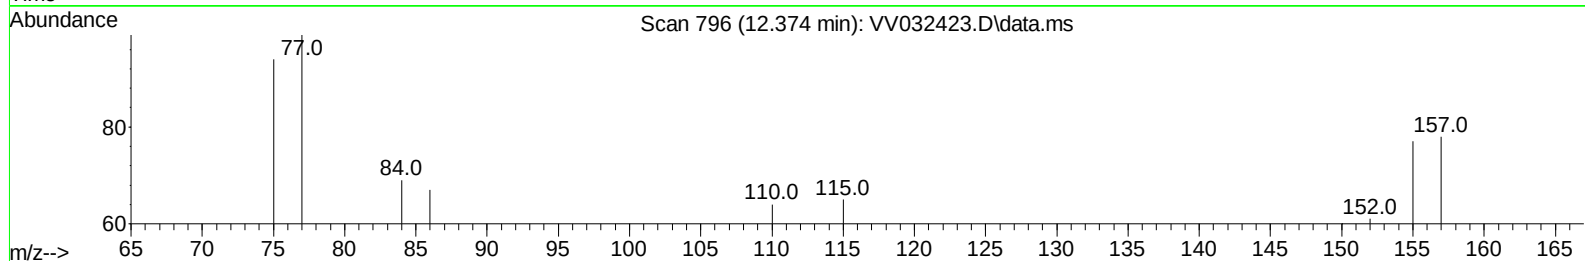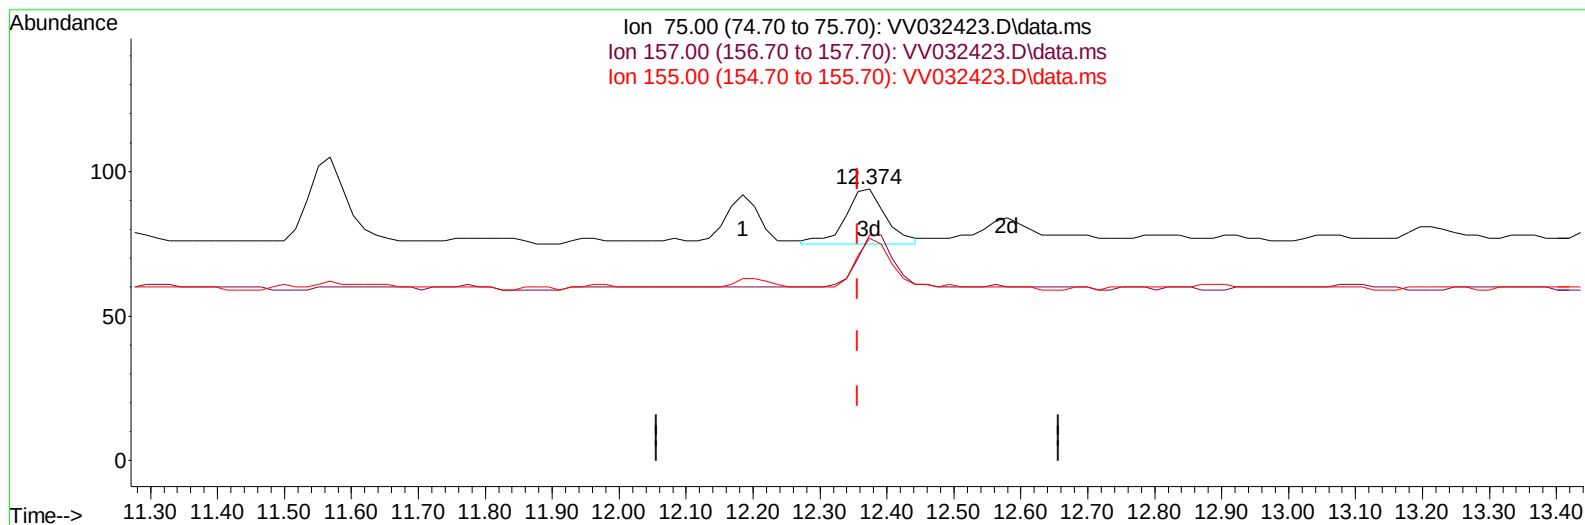

TIC: VV032423.D\data.ms

(13) 1,2-Dibromo-3-chloropropane (T)

12.374min (+ 0.017) 0.11 ug/L m

response 79

Ion	Exp%	Act%
75.00	100.00	100.00
157.00	76.30	82.98
155.00	67.80	81.91#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101323\
 Data File : VV032423.D
 Acq On : 13 Oct 2023 11:58
 Operator : SY/MD
 Sample : VSTD0.140
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1240

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/16/2023
 Supervised By :Semsettin Yesilyurt 10/16/2023

Quant Time: Oct 16 02:45:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101323.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 16 02:44:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6657	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6474	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	3582	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	1034	0.095	ug/L	0.00
4) 1,2-Dichloroethane-d4	4.969	65	667	0.097	ug/L	0.02
7) 1,2-Dichloropropane-d6	5.995	67	828	0.093	ug/L	0.00
8) Toluene-d8	7.253	98	1989	0.094	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.146	84	588	0.096	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.280	62	792	0.100	ug/L	87
6) Trichloroethene	5.852	95	694	0.100	ug/L	95
9) 1,2-Dibromoethane	8.305	107	452	0.101	ug/L #	88
12) 1,2,3-Trichloropropane	10.214	75	422	0.102	ug/L	98
13) 1,2-Dibromo-3-chloropr...	12.374	75	79m	0.114	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101323\
Data File : VV032423.D
Acq On : 13 Oct 2023 11:58
Operator : SY/MD
Sample : VSTD0.140
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1240

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/16/2023
Supervised By :Semsettin Yesilyurt 10/16/2023

Quant Time: Oct 16 02:45:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101323.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 16 02:44:39 2023
Response via : Initial Calibration

