

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101419\
 Data File : VV013146.D
 Acq On : 14 Oct 2019 17:15
 Operator : SY/MD
 Sample : K5347-04DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 15 05:11:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 15 05:07:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	734878	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	695835	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	249211	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	185927	40.03	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.06%
7) Chloroethane-d5	1.58	69	165843	43.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.10%
11) 1,1-Dichloroethene-d2	2.13	63	248041	28.31	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	56.62%#
21) 2-Butanone-d5	3.97	46	360393	103.18	ug/L	0.06
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.18%
24) Chloroform-d	4.40	84	416509	46.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.16%
26) 1,2-Dichloroethane-d4	5.08	65	270159	49.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.02%
32) Benzene-d6	5.10	84	862269	46.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.90%
36) 1,2-Dichloropropane-d6	6.12	67	278073	47.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.62%
41) Toluene-d8	7.36	98	724785	43.63	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.26%
43) trans-1,3-Dichloropropene-	7.66	79	113458	43.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.12%
47) 2-Hexanone-d5	8.14	63	204210	88.24	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.24%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	338834	45.14	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.28%
64) 1,2-Dichlorobenzene-d4	11.67	152	256848	52.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.20%


Target Compounds					Ovalue
46) Tetrachloroethene	8.02	164	290438	65.011 ug/L	97
48) 2-Hexanone	8.14	43	26005	4.681 ug/L #	77
59) 1,2,3-Trichloropropane	11.29	75	27270	4.082 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101419\
Data File : VV013146.D
Acq On : 14 Oct 2019 17:15
Operator : SY/MD
Sample : K5347-04DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 15 05:11:02 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 15 05:07:22 2019
Response via : Initial Calibration




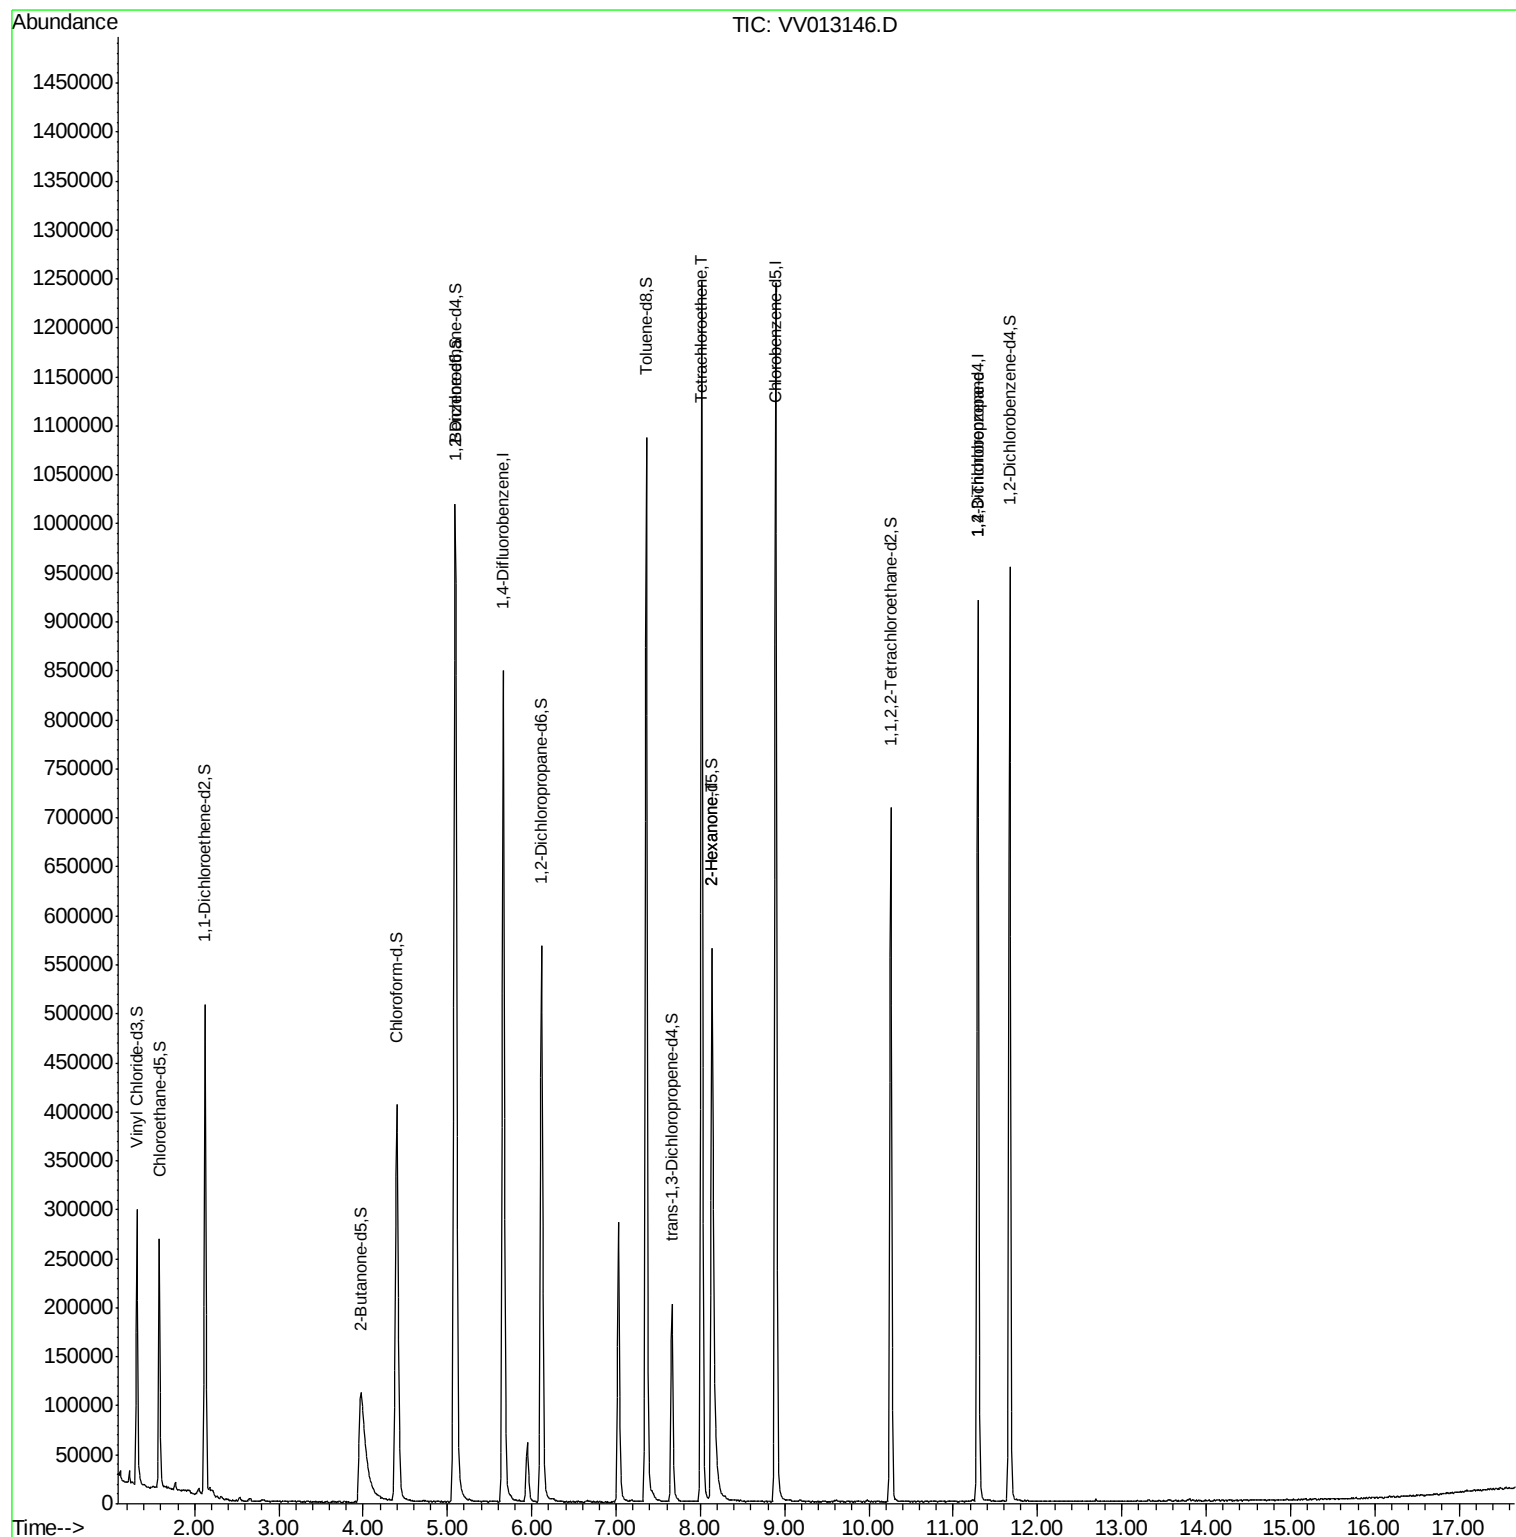


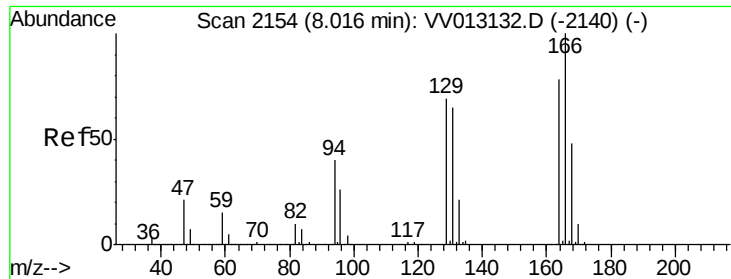

#46
Tetrachloroethene
Concen: 65.011 ug/L
RT: 8.02 min Scan# 2154
Delta R.T. 0.00 min
Lab File: VV013146.D
Acq: 14 Oct 2019 17:15




Instrument :
MSVOA_V
ClientSampleId :


Tot Ion:	164	Resp:	290438
Ion	Ratio	Lower	Upper
164	100		
129	86.9	63.1	117.1
131	83.7	62.4	116.0
166	128.7	91.3	169.6

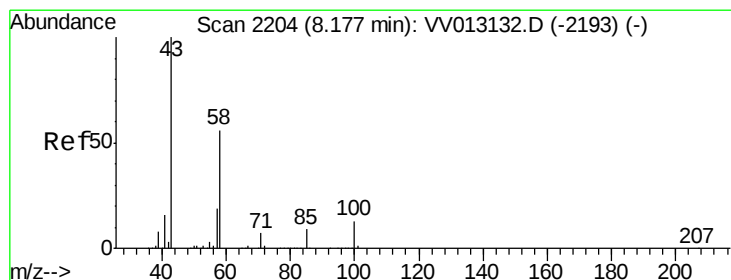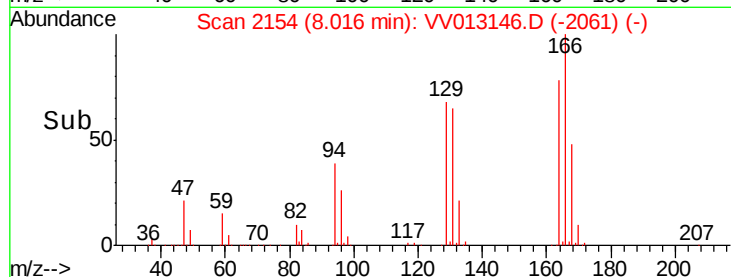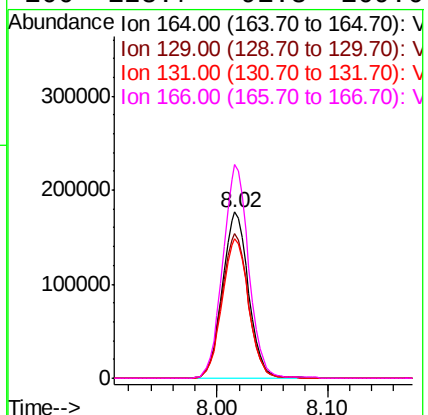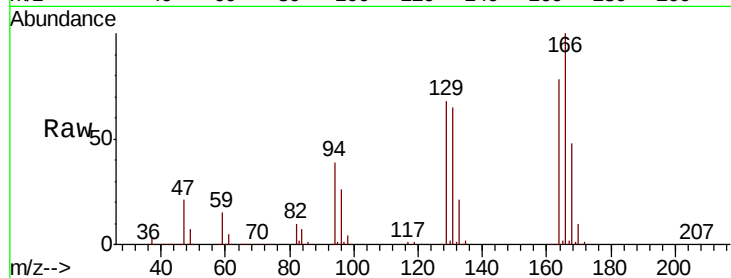

#48
2-Hexanone
Concen: 4.681 ug/L
RT: 8.14 min Scan# 2192
Delta R.T. -0.04 min
Lab File: VV013146.D
Acq: 14 Oct 2019 17:15

Tgt Ion:	43	Resp:	26005
Ion	Ratio	Lower	Upper
43	100		
58	41.4	44.9	67.3#
57	32.4	15.0	22.6#
100	3.6	10.2	15.2#

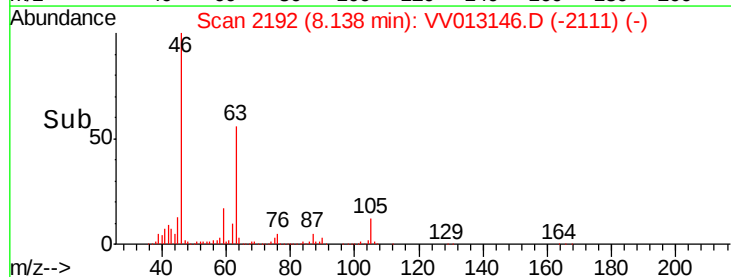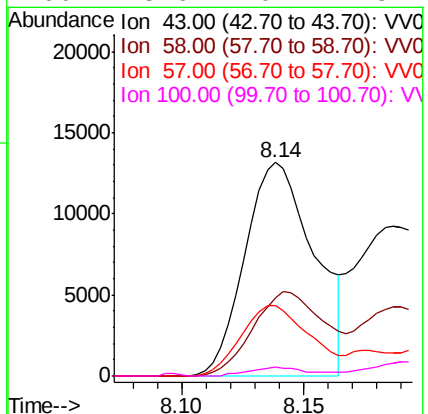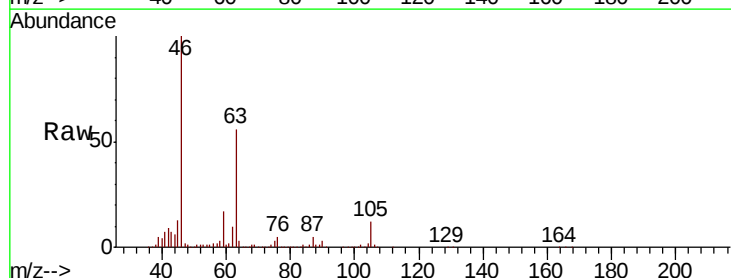

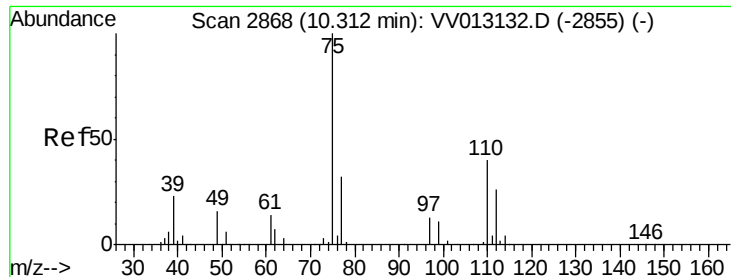

#59

1,2,3-Trichloropropane

Concen: 4.082 ug/L

RT: 11.29 min Scan# 3172

Delta R.T. 0.98 min

Lab File: VV013146.D

Acq: 14 Oct 2019 17:15

Instrument :

MSVOA_V

ClientSampleId :

Tot Ion: 75 Resp: 27270

Ion Ratio Lower Upper

75 100

77 36.5 25.7 38.5

