


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV0101419\
Data File : VV013131.D
Acq On : 14 Oct 2019 09:12
Operator : SY/MD
Sample : BFB72
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
Title : VOC Analysis
Last Update : Wed Oct 16 10:30:20 2019

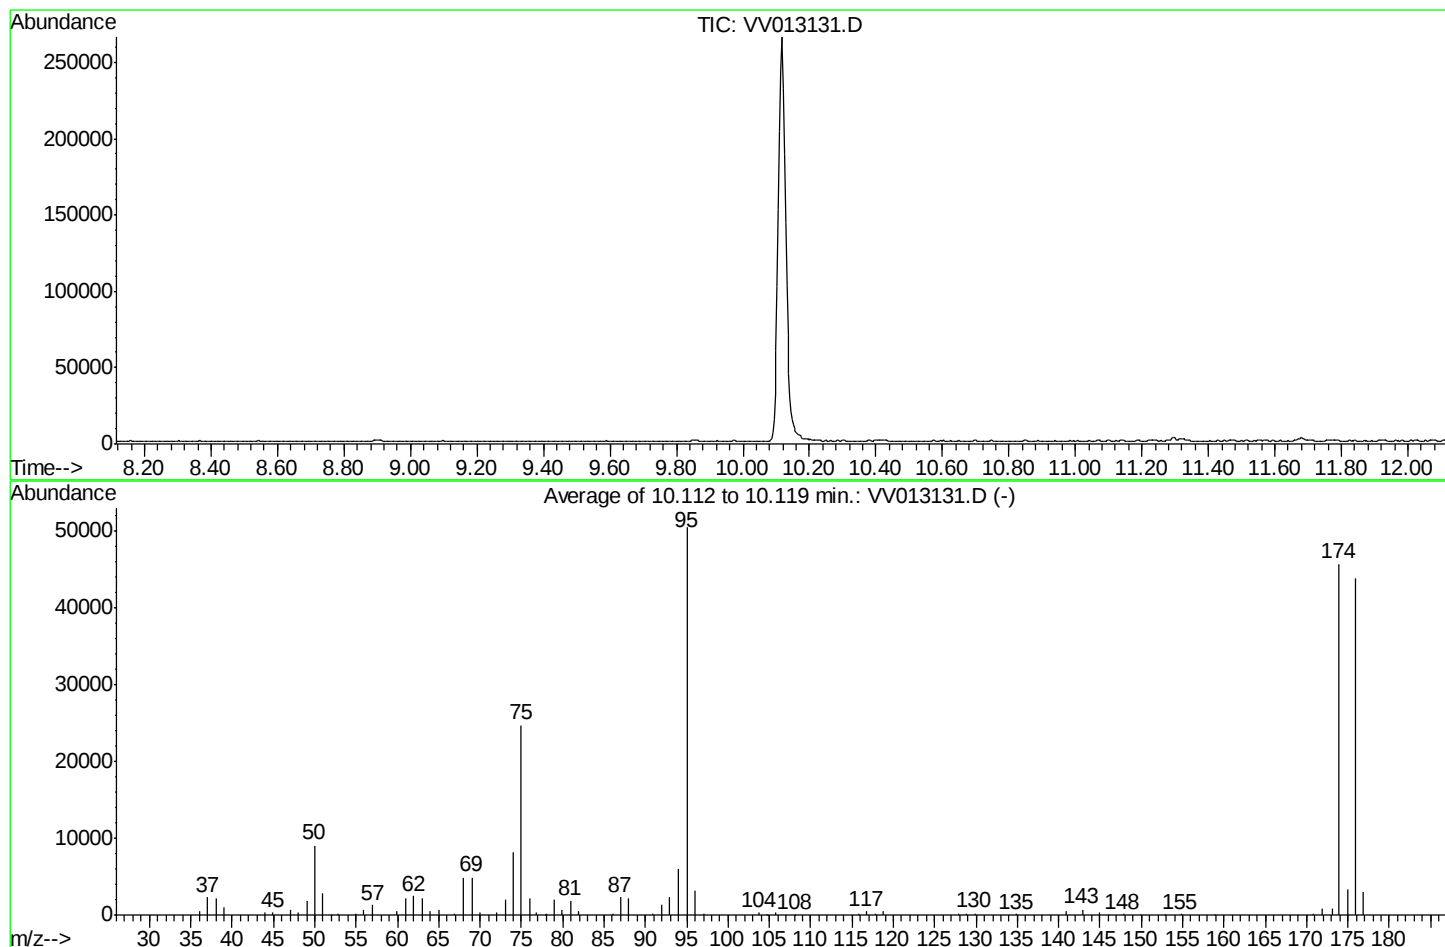

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	9008	PASS
75	95	30	80	49.0	24709	PASS
95	95	100	100	100.0	50474	PASS
96	95	5	9	6.4	3220	PASS
173	174	0.00	2	1.7	771	PASS
174	95	50	120	90.5	45672	PASS
175	174	5	9	7.4	3361	PASS
176	174	95	101	95.8	43765	PASS
177	176	5	9	6.7	2946	PASS

m/z	Abundance
36.00	523.0
37.00	2291.0
38.00	2262.0
39.00	1112.0
40.00	847.0
44.00	1039.0
44.90	280.0
47.10	578.0
48.00	373.0
49.00	1895.0
50.00	8806.0
51.00	2768.0
52.00	107.0
52.80	110.0
55.00	181.0
56.00	711.0
57.00	1340.0
59.90	433.0
61.00	2067.0
62.00	2378.0
63.00	2066.0
63.90	537.0
65.00	572.0
66.80	140.0
68.00	4444.0
69.00	4755.0
69.90	386.0
72.00	278.0
73.00	1934.0
74.00	8156.0
75.00	23768.0
76.00	2332.0
76.90	335.0
78.10	262.0
78.90	1961.0
79.90	672.0
80.90	1859.0
81.80	544.0
86.10	262.0
87.00	2111.0
87.90	2112.0
90.90	182.0
92.00	1308.0
92.90	2329.0
94.00	5535.0
95.00	48560.0
96.00	3229.0
97.00	107.0
103.80	248.0
105.70	224.0
115.90	247.0
116.80	416.0
117.80	148.0
118.80	404.0
128.00	197.0
128.80	103.0
129.80	171.0
134.90	149.0
140.90	529.0
142.90	688.0
144.90	382.0
147.70	120.0
152.90	122.0
154.80	169.0
170.80	253.0
171.90	794.0
173.10	790.0
173.90	42216.0
174.90	3222.0
175.90	40712.0
176.90	2764.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.00	589.0
37.00	2411.0
38.00	2306.0
39.00	1116.0
39.90	847.0
44.00	993.0
44.90	296.0
47.10	675.0
48.00	419.0
49.00	1913.0
50.00	9272.0
51.00	3016.0
52.80	138.0
55.00	155.0
56.00	747.0
57.00	1374.0
60.00	454.0
61.00	2162.0
62.00	2630.0
63.00	2257.0
63.90	550.0
65.10	746.0
66.80	144.0
68.00	4918.0
69.00	5065.0
69.90	404.0
72.00	333.0
73.00	2126.0
74.00	8537.0
75.00	25656.0
76.00	2285.0
76.80	343.0
78.10	246.0
78.90	2105.0
79.90	775.0
80.90	1912.0
81.80	604.0
86.10	208.0
86.90	2374.0
87.90	2281.0
90.90	223.0
92.00	1337.0
92.90	2341.0
94.00	6220.0
95.00	52240.0
96.00	3312.0
97.00	112.0
103.80	273.0
105.80	274.0
108.10	109.0
115.90	225.0
116.80	466.0
117.80	169.0
118.80	432.0
127.90	167.0
128.80	152.0
129.80	204.0
134.90	133.0
140.90	541.0
142.90	703.0
144.90	392.0
146.00	110.0
147.80	128.0
152.90	103.0
154.80	128.0
158.80	110.0
170.90	243.0
171.90	898.0
173.00	796.0
173.90	47120.0
174.90	3463.0
175.90	45160.0
176.90	3004.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.00	529.0
37.00	2291.0
38.00	2101.0
39.00	979.0
39.90	900.0
44.00	990.0
45.00	310.0
47.10	683.0
48.00	447.0
49.10	1889.0
50.00	8948.0
51.00	2980.0
52.90	142.0
55.00	123.0
55.90	687.0
57.00	1246.0
60.00	459.0
61.00	2237.0
62.00	2411.0
63.00	2223.0
64.00	557.0
65.00	828.0
66.90	118.0
68.00	5010.0
69.00	4929.0
69.90	394.0
72.00	343.0
73.00	2113.0
74.00	7964.0
75.00	24704.0
76.00	2090.0
76.70	306.0
77.80	223.0
78.90	1902.0
79.90	720.0
80.90	1731.0
81.90	560.0
86.10	138.0
86.90	2332.0
88.00	1993.0
90.80	232.0
92.00	1313.0
92.90	2240.0
94.00	6186.0
95.00	50624.0
96.00	3119.0
97.00	102.0
103.80	284.0
104.60	114.0
105.90	290.0
108.10	105.0
115.80	202.0
116.80	458.0
117.80	168.0
118.80	434.0
127.80	157.0
128.80	165.0
129.90	191.0
134.90	101.0
140.90	464.0
142.90	742.0
145.00	359.0
146.00	120.0
147.90	125.0
149.90	115.0
158.80	113.0
170.80	188.0
171.90	984.0
173.00	729.0
173.90	47680.0
175.00	3398.0
175.90	45424.0
176.90	3071.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Scan 2795 (10.077 min): VV013131.D
BFB72

m/z	Abundance
39.90	980.0
42.90	109.0
44.00	737.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72