

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101420\
 Data File : VV018903.D
 Acq On : 14 Oct 2020 19:08
 Operator : SY/MD
 Sample : L4382-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG409

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 10:58:43 AM

Quant Time: Oct 15 02:09:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 02:07:27 2020
 Response via : Initial Calibration

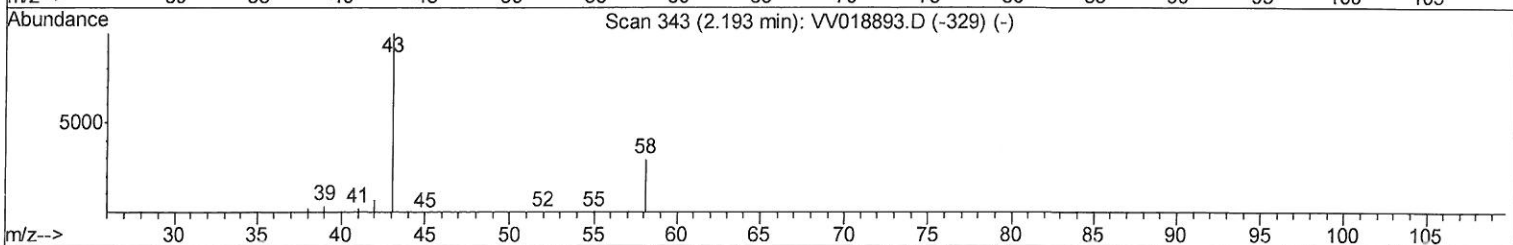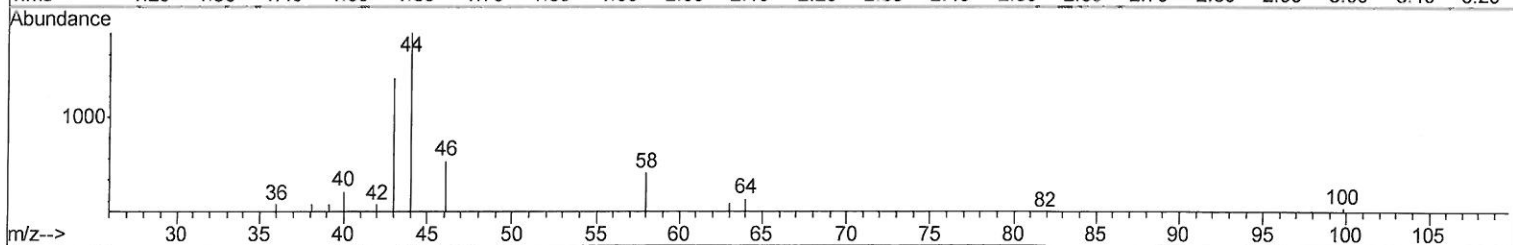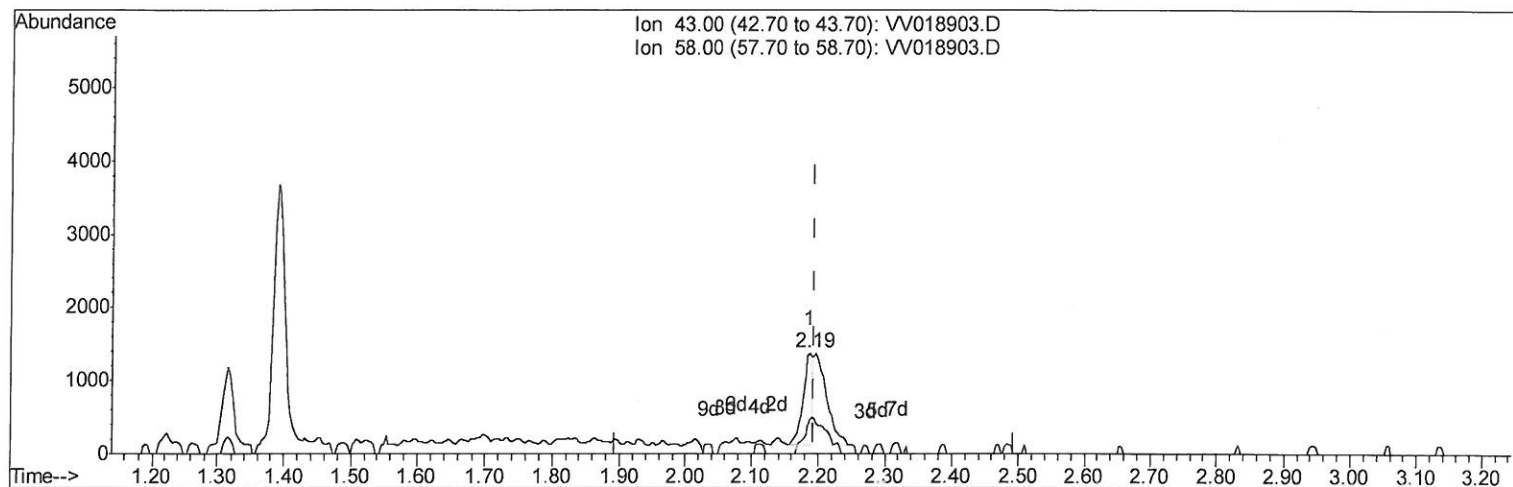

TIC: VV018903.D

(13) Acetone (T)
 2.187min (-0.006) 1.02ug/L
 response 1232

Ion	Exp%	Act%
43.00	100	100
58.00	29.40	86.04#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101420\
 Data File : VV018903.D
 Acq On : 14 Oct 2020 19:08
 Operator : SY/MD
 Sample : L4382-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG409

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 10:58:43 AM

Quant Time: Oct 15 02:09:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 02:07:27 2020
 Response via : Initial Calibration

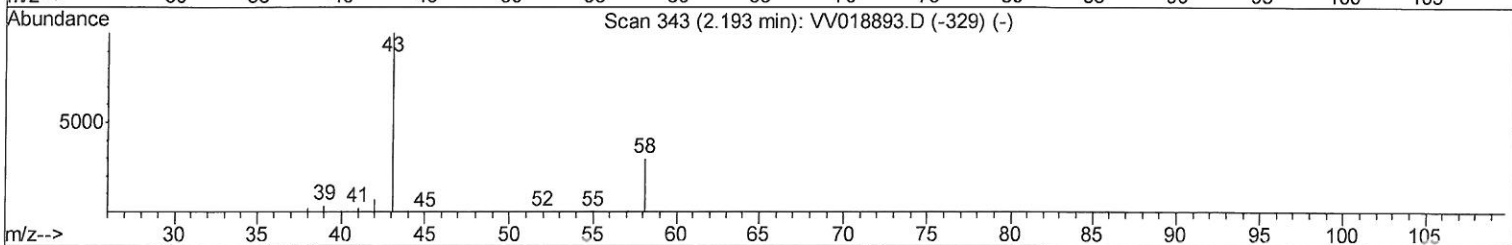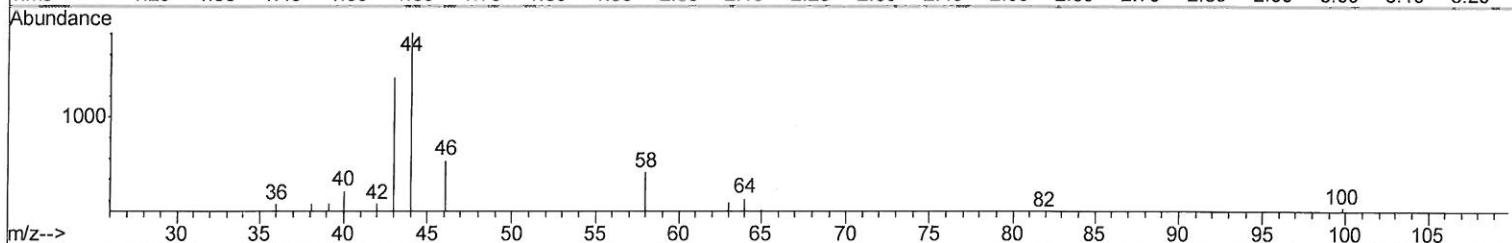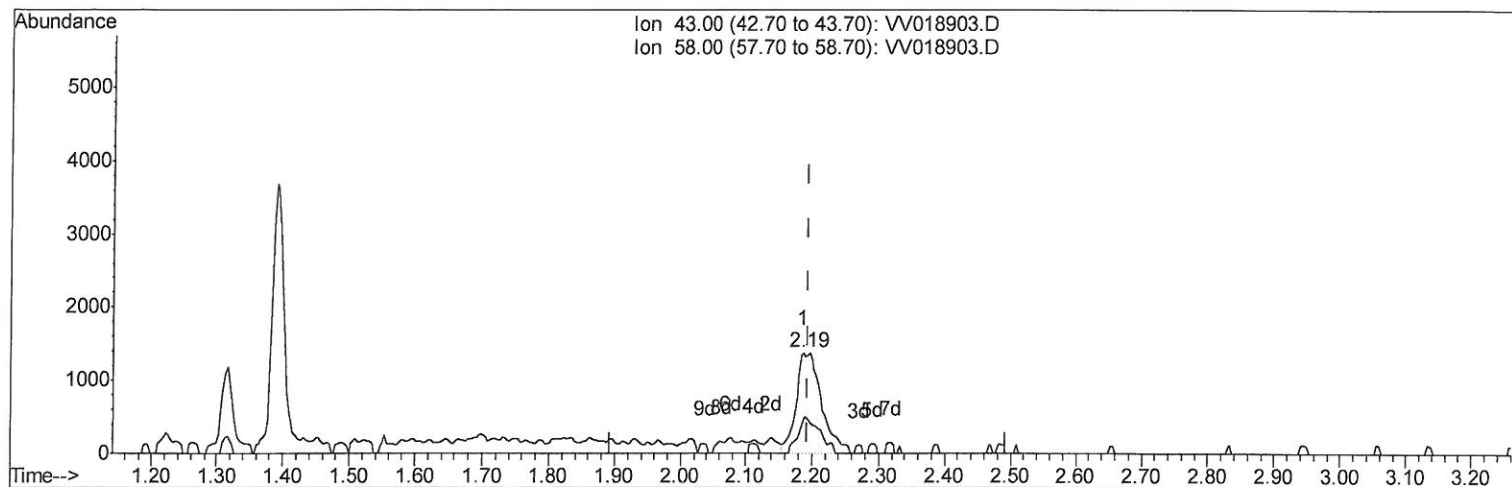

TIC: VV018903.D

(13) Acetone (T)

2.187min (-0.006) 3.03ug/L m

210/27/10 dy

response 3658

Ion	Exp%	Act%
43.00	100	100
58.00	29.40	28.98
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101420\
 Data File : VV018903.D
 Acq On : 14 Oct 2020 19:08
 Operator : SY/MD
 Sample : L4382-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG409

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 10:58:43 AM

Quant Time: Oct 15 03:34:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 02:07:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	288311	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	286816	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	133646	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	122461	51.60	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	103.20%
7) Chloroethane-d5	1.58	69	100317	53.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.70%
11) 1,1-Dichloroethene-d2	2.12	63	180743	40.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.68%
21) 2-Butanone-d5	3.91	46	151587	91.64	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.64%
24) Chloroform-d	4.37	84	218379	51.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.42%
26) 1,2-Dichloroethane-d4	5.05	65	153301	54.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.32%
32) Benzene-d6	5.07	84	446827	53.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.72%
36) 1,2-Dichloropropane-d6	6.09	67	145882	54.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.98%
41) Toluene-d8	7.34	98	389270	51.82	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.64%
43) trans-1,3-Dichloropropene-	7.64	79	66653	50.94	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.88%
47) 2-Hexanone-d5	8.11	63	80251	80.70	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.70%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	138580	44.17	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.34%
64) 1,2-Dichlorobenzene-d4	11.65	152	153630	56.50	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.00%

Target Compounds

13) Acetone	2.19	43	3658m	Ovalue	3.026 ug/L
-------------	------	----	-------	--------	------------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101420\
Data File : VV018903.D
Acq On : 14 Oct 2020 19:08
Operator : SY/MD
Sample : L4382-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG409

Manual Integrations
APPROVED

MMDadoda
10/19/2020 10:58:43 AM

Quant Time: Oct 15 03:34:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 15 02:07:27 2020
Response via : Initial Calibration

