


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV101420\
 Data File : VV018890.D
 Acq On : 14 Oct 2020 09:42
 Operator : SY/MD
 Sample : BFB74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB74

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 15 02:07:27 2020

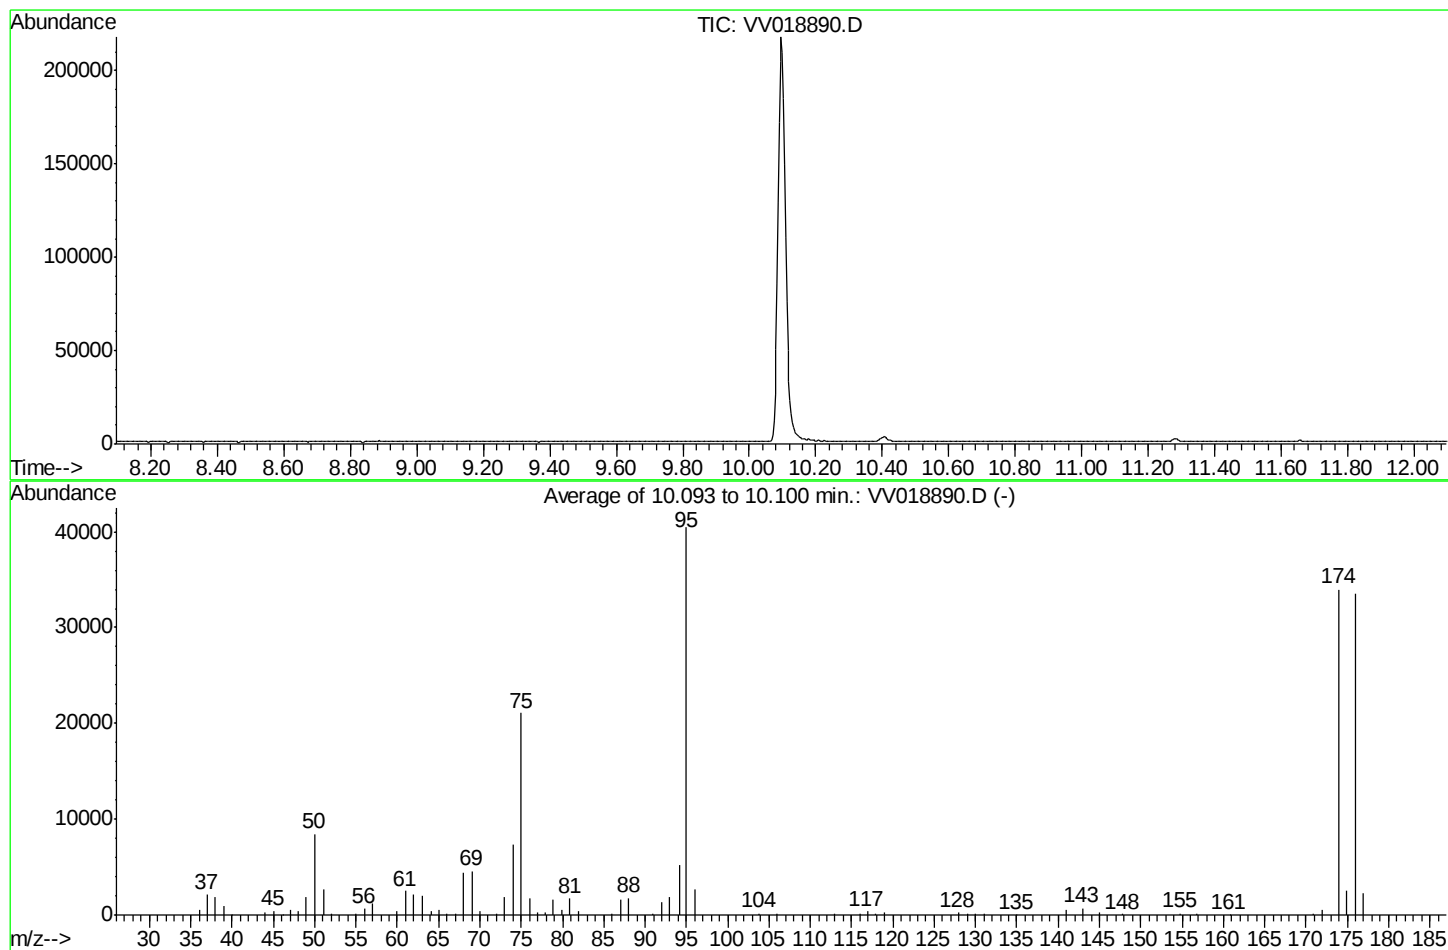

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	8486	PASS
75	95	30	80	52.1	21101	PASS
95	95	100	100	100.0	40466	PASS
96	95	5	9	6.5	2636	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.9	33970	PASS
175	174	5	9	7.5	2558	PASS
176	174	95	101	98.9	33592	PASS
177	176	5	9	6.8	2289	PASS

m/z	Abundance
36.00	572.0
37.00	2206.0
38.00	1808.0
39.00	899.0
39.90	262.0
44.00	1257.0
45.00	463.0
46.20	119.0
47.00	477.0
47.90	397.0
49.00	1709.0
50.00	8469.0
51.10	2700.0
52.10	216.0
55.00	118.0
56.00	633.0
57.00	1175.0
59.90	413.0
61.00	2583.0
62.00	2119.0
63.00	2031.0
64.00	442.0
65.00	560.0
65.90	118.0
67.00	245.0
68.00	4201.0
69.00	4423.0
70.00	346.0
72.00	182.0
73.00	1853.0
74.00	7535.0
75.00	20320.0
76.10	1668.0
76.90	271.0
78.00	274.0
78.90	1469.0
80.00	497.0
80.90	1759.0
81.90	386.0
86.00	131.0
87.00	1602.0
88.00	1809.0
90.90	147.0
92.00	1455.0
93.00	1746.0
94.10	4950.0
95.00	39552.0
96.00	2651.0
103.80	175.0
106.00	191.0
113.00	115.0
115.90	199.0
116.90	435.0
117.90	186.0
118.90	317.0
127.90	209.0
129.00	105.0
131.00	114.0
134.90	107.0
140.90	551.0
142.90	646.0
144.90	252.0
147.80	131.0
154.70	146.0
170.90	108.0
171.90	529.0
174.00	32792.0
174.90	2381.0
176.00	31760.0
177.00	2275.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.00	555.0
37.00	2147.0
38.00	1873.0
39.00	950.0
39.90	218.0
44.00	1340.0
45.00	466.0
47.00	551.0
48.00	370.0
49.00	1963.0
50.00	8830.0
51.10	2719.0
52.00	199.0
54.90	128.0
56.00	646.0
57.00	1201.0
60.00	430.0
61.00	2617.0
62.00	2258.0
63.00	2066.0
64.00	420.0
65.00	587.0
65.90	138.0
67.00	190.0
68.00	4601.0
69.00	4805.0
70.00	405.0
72.00	205.0
73.00	1958.0
74.00	7648.0
75.00	22040.0
76.10	1785.0
76.90	274.0
78.00	287.0
78.90	1624.0
79.90	534.0
80.90	1782.0
81.90	371.0
86.00	212.0
87.00	1724.0
88.00	1813.0
90.90	143.0
92.00	1475.0
93.00	1997.0
94.10	5369.0
95.00	41624.0
96.00	2725.0
103.80	198.0
106.00	207.0
113.00	119.0
116.00	208.0
116.90	399.0
117.90	188.0
118.90	334.0
127.90	261.0
129.00	129.0
130.00	114.0
131.00	137.0
140.90	586.0
143.00	694.0
145.00	241.0
147.90	125.0
154.80	178.0
156.80	134.0
170.90	111.0
171.90	555.0
174.00	34984.0
174.90	2619.0
176.00	34800.0
177.00	2368.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.00	439.0
37.00	1938.0
38.00	1827.0
39.00	953.0
39.90	198.0
44.00	1390.0
45.00	440.0
47.00	565.0
48.00	288.0
49.00	1945.0
50.00	8160.0
51.10	2536.0
52.00	181.0
54.90	161.0
56.00	624.0
57.00	1201.0
60.00	440.0
61.00	2401.0
62.00	2175.0
63.00	1931.0
64.10	397.0
65.00	538.0
65.90	130.0
66.90	137.0
68.00	4553.0
69.00	4542.0
70.00	403.0
72.00	203.0
73.00	1900.0
74.00	7054.0
75.00	20944.0
76.10	1734.0
76.90	239.0
77.90	242.0
78.90	1667.0
79.90	536.0
80.90	1659.0
81.90	348.0
86.00	234.0
87.00	1614.0
88.00	1633.0
91.00	147.0
92.00	1260.0
93.00	1985.0
94.10	5187.0
95.00	40224.0
96.00	2532.0
103.90	242.0
106.00	197.0
116.00	192.0
116.90	342.0
117.80	194.0
118.90	310.0
127.90	247.0
129.00	103.0
129.90	132.0
131.00	110.0
135.00	105.0
140.90	511.0
142.90	691.0
145.00	215.0
147.90	101.0
154.90	204.0
156.80	147.0
160.80	123.0
171.90	567.0
174.00	34136.0
174.90	2674.0
176.00	34216.0
177.00	2224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

Scan 2789 (10.058 min): VV018890.D
BFB74

m/z	Abundance
39.90	213.0
44.00	1100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74