


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022783.D
Acq On : 14 Oct 2021 11:31
Operator : SY/MD
Sample : M4167-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YATK9

Manual Integrations
APPROVED

MMDadoda
10/15/2021 12:02:48 PM

Quant Time: Oct 15 01:58:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 01:58:00 2021
Response via : Initial Calibration

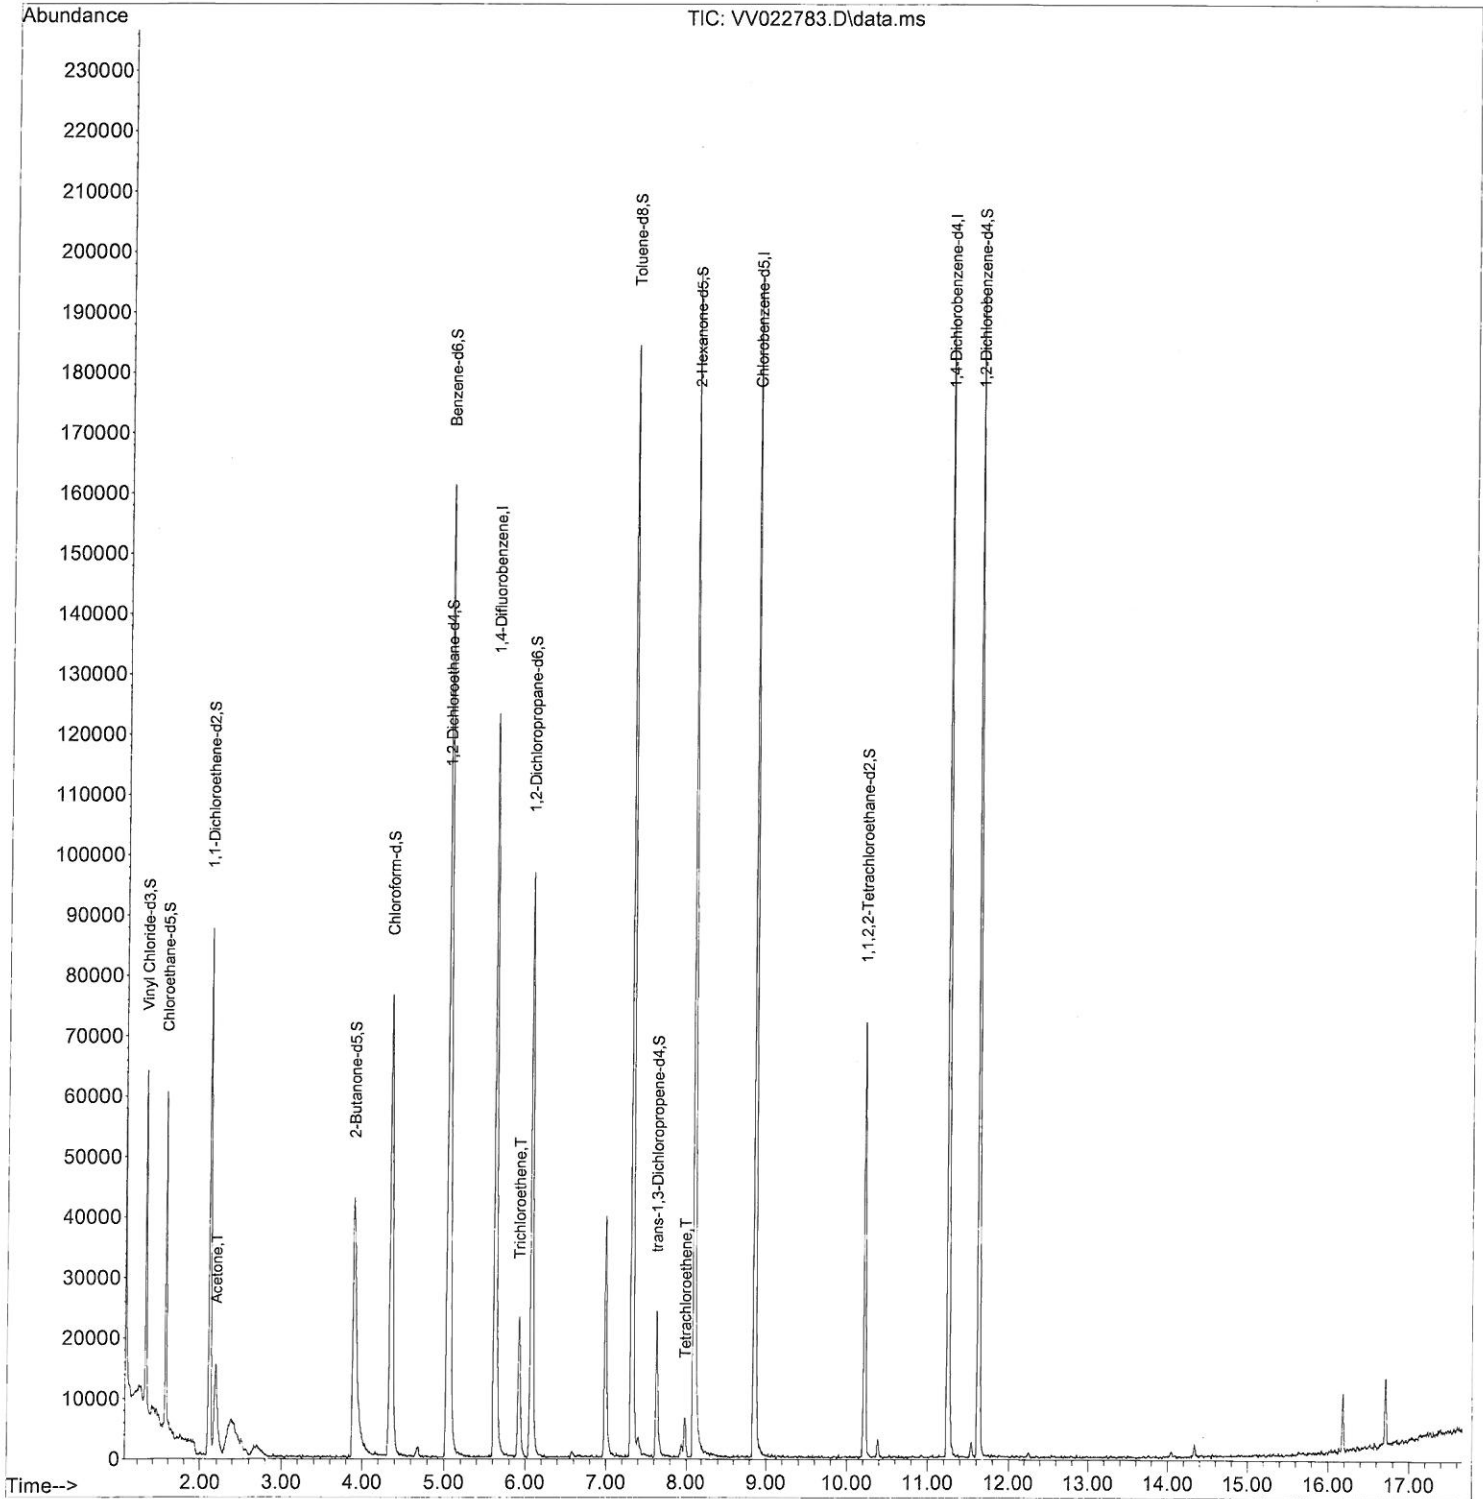

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022783.D
 Acq On : 14 Oct 2021 11:31
 Operator : SY/MD
 Sample : M4167-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YATK9

Manual Integrations
 APPROVED

MMDadoda
 10/15/2021 12:02:48 PM

Quant Time: Oct 15 01:58:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 15 01:58:00 2021
 Response via : Initial Calibration

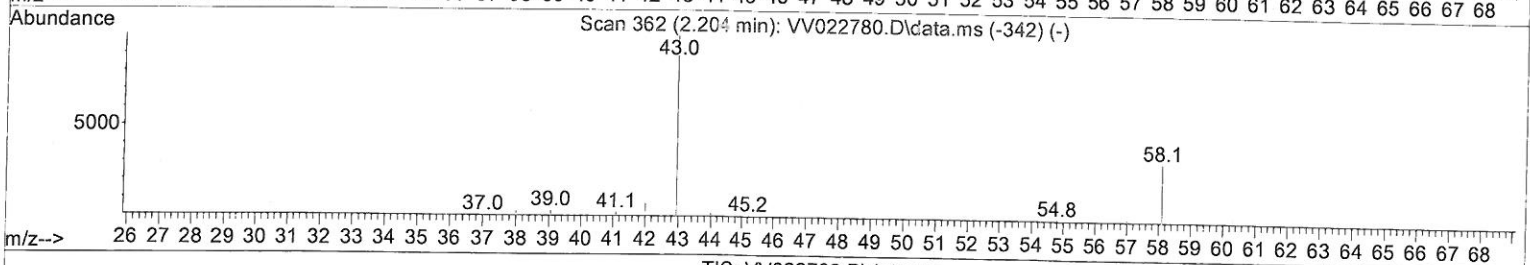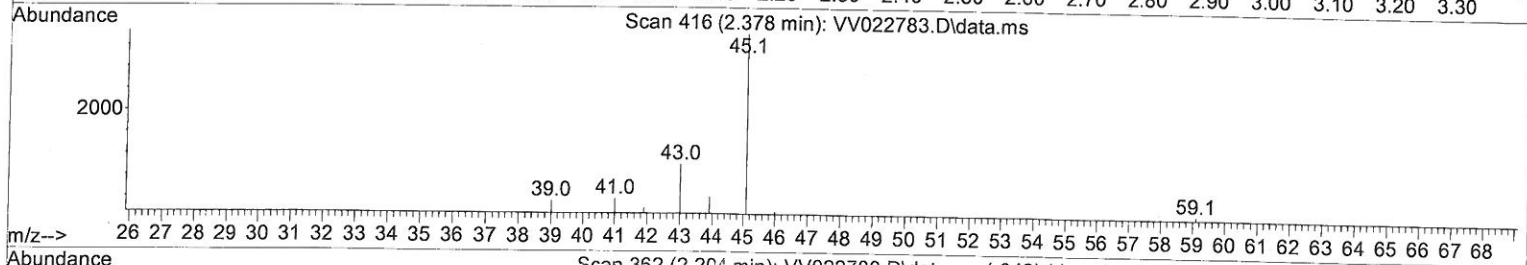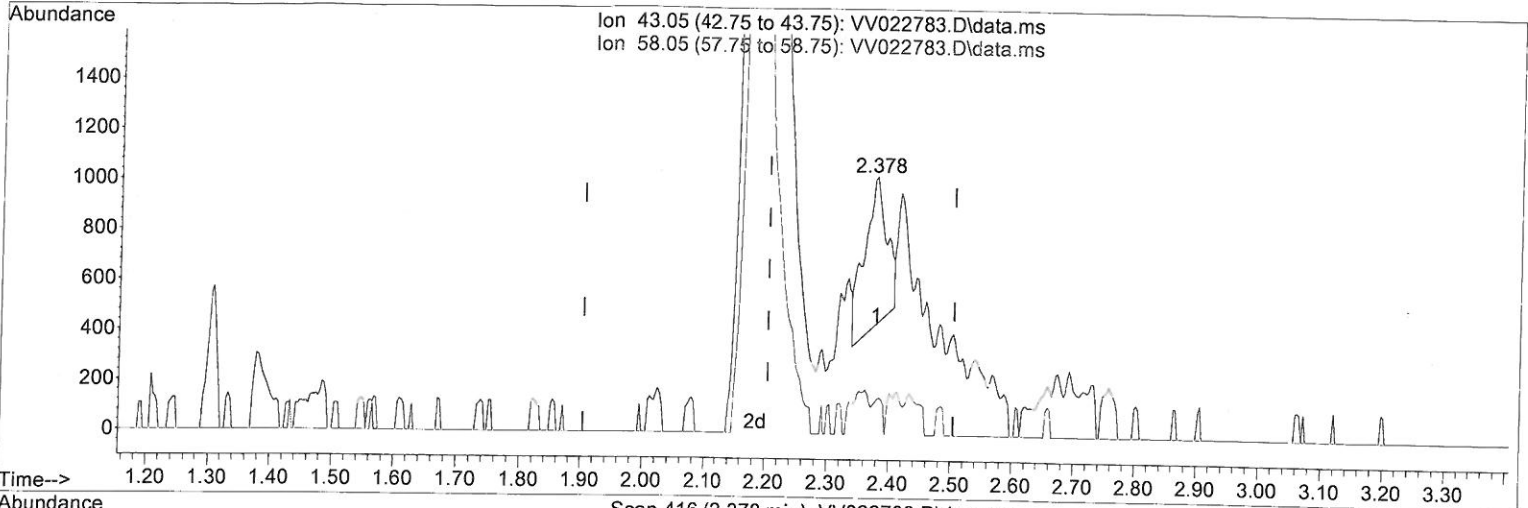

TIC: VV022783.D\data.ms

(13) Acetone (T)

2.378min (+ 0.174) 1.33 ug/L

response 1476

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	24.19
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022783.D
Acq On : 14 Oct 2021 11:31
Operator : SY/MD
Sample : M4167-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YATK9

Manual Integrations
APPROVED

MMDadoda
10/15/2021 12:02:48 PM

Quant Time: Oct 15 01:58:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 01:58:00 2021
Response via : Initial Calibration

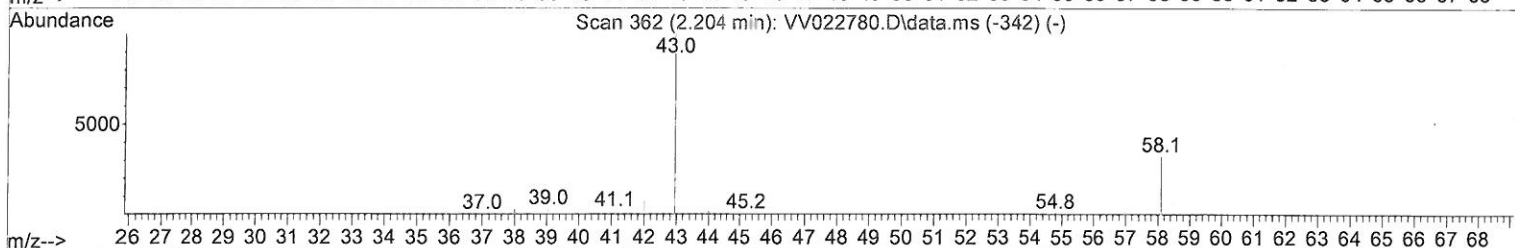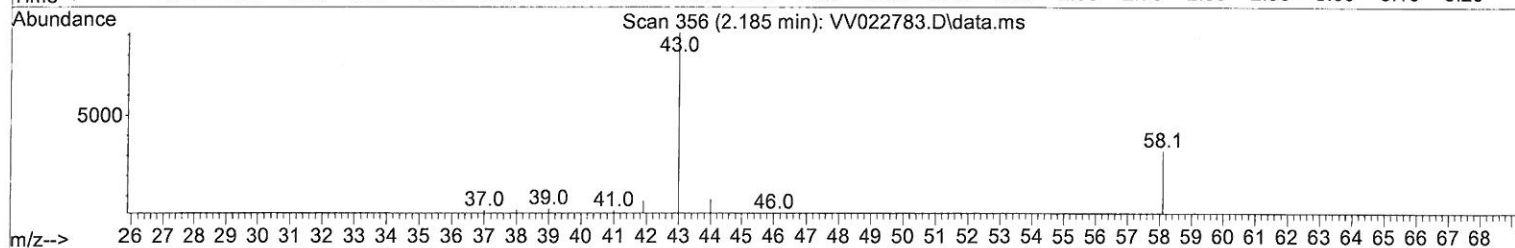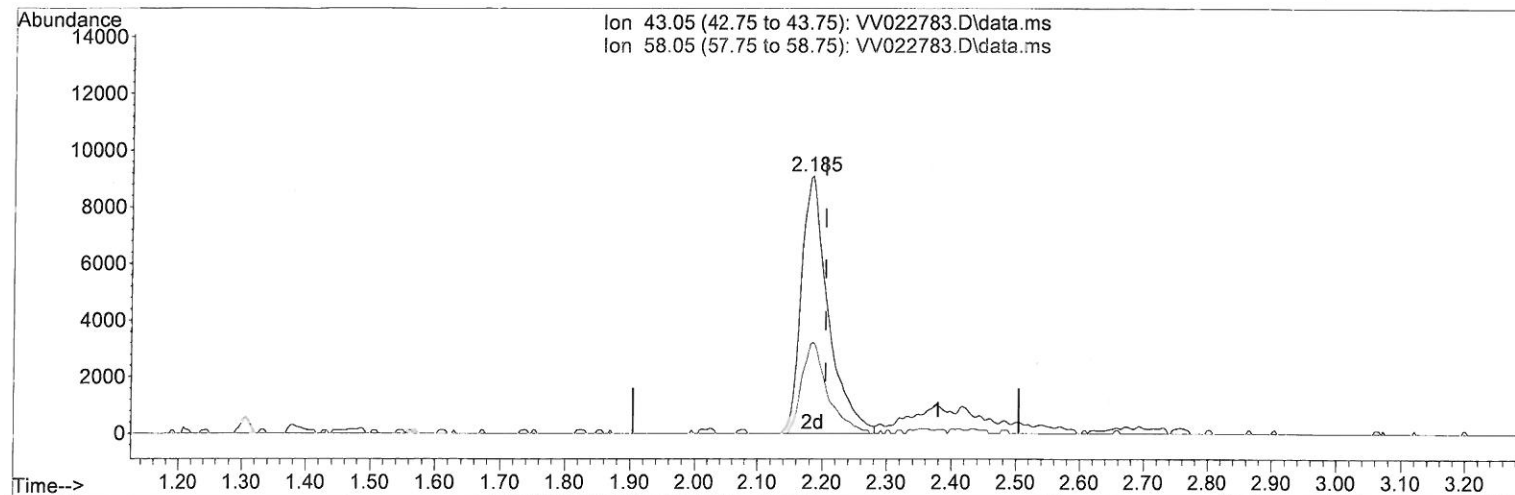

TIC: VV022783.D\data.ms

(13) Acetone (T)

2.185min (-0.019) 23.80 ug/L m

response 26414

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	1.35
0.00	0.00	0.00
0.00	0.00	0.00

7MD
10/22/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022783.D
 Acq On : 14 Oct 2021 11:31
 Operator : SY/MD
 Sample : M4167-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YATK9

Manual Integrations
 APPROVED

MMDadoda
 10/15/2021 12:02:48 PM

Quant Time: Oct 15 01:58:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 15 01:58:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	110306	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	113831	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	52975	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	32605	4.296	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	86.000%		
7) Chloroethane-d5	1.564	69	33605	4.928	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	98.600%		
11) 1,1-Dichloroethene-d2	2.108	63	45099	3.029	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	60.600%		
20) 2-Butanone-d5	3.892	46	83700	42.062	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	84.120%		
24) Chloroform-d	4.349	84	80950	5.176	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	103.600%		
26) 1,2-Dichloroethane-d4	5.034	65	36233	4.773	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	95.400%		
32) Benzene-d6	5.050	84	149163	4.402	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	88.000%		
36) 1,2-Dichloropropane-d6	6.072	67	48358	4.819	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	96.400%		
41) Toluene-d8	7.320	98	123795	4.226	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	84.600%		
43) trans-1,3-Dichloroprop...	7.625	79	14789	4.442	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	88.800%		
46) 2-Hexanone-d5	8.092	63	66838	49.820	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	99.640%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34412	5.062	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	101.200%		
66) 1,2-Dichlorobenzene-d4	11.625	152	50279	5.119	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	102.400%		
Target Compounds						
13) Acetone	2.185	43	26414m	23.805	ug/L	Qvalue
34) Trichloroethene	5.918	95	8457	1.014	ug/L	94
47) Tetrachloroethene	7.979	164	1526	0.226	ug/L	93

9m9
 10/22/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed