


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022784.D
Acq On : 14 Oct 2021 11:55
Operator : SY/MD
Sample : M4167-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YATLO

Manual Integrations
APPROVED

MMDadoda
10/15/2021 12:02:52 PM

Quant Time: Oct 15 01:59:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 01:58:00 2021
Response via : Initial Calibration

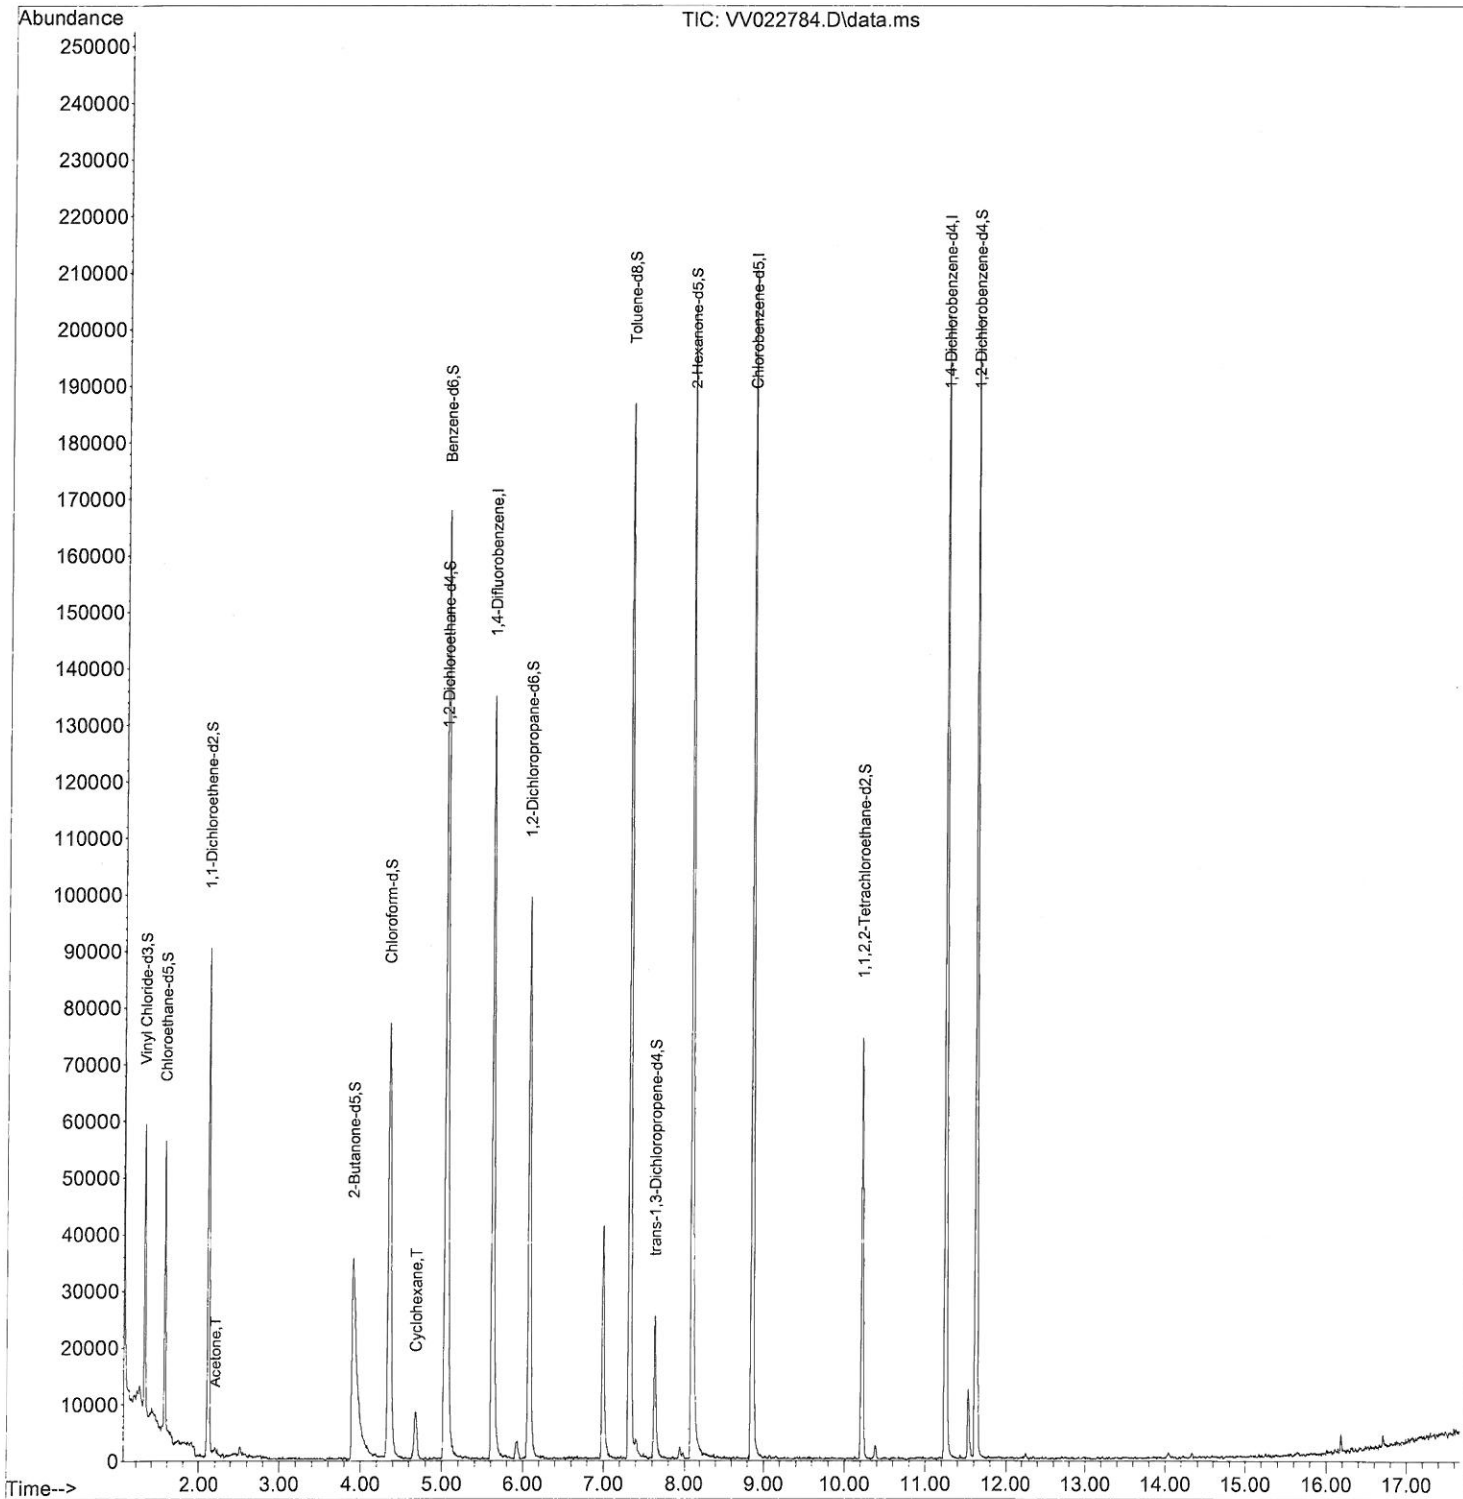

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022784.D
Acq On : 14 Oct 2021 11:55
Operator : SY/MD
Sample : M4167-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YATLO

Manual Integrations
APPROVED

MMDadoda
10/15/2021 12:02:52 PM

Quant Time: Oct 15 01:59:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 01:58:00 2021
Response via : Initial Calibration

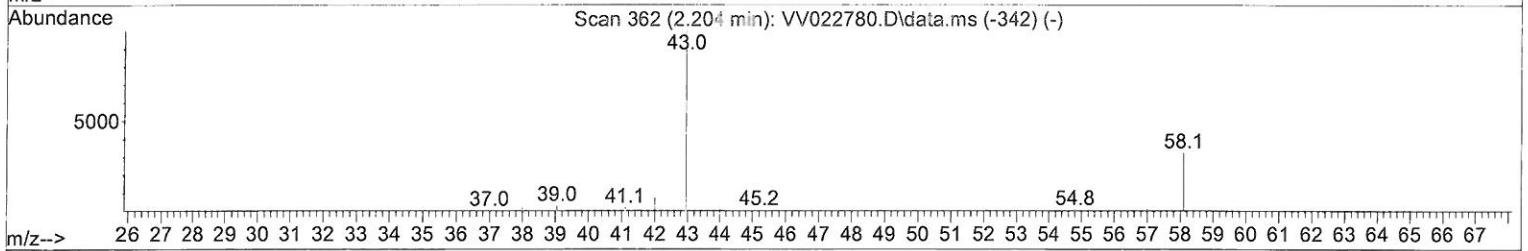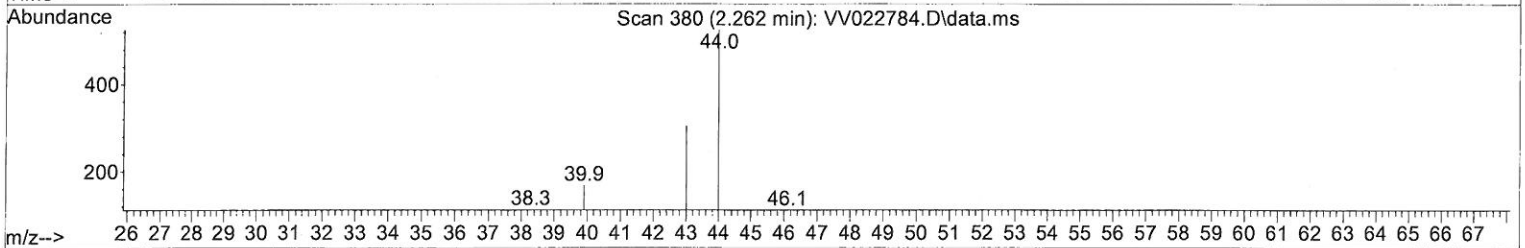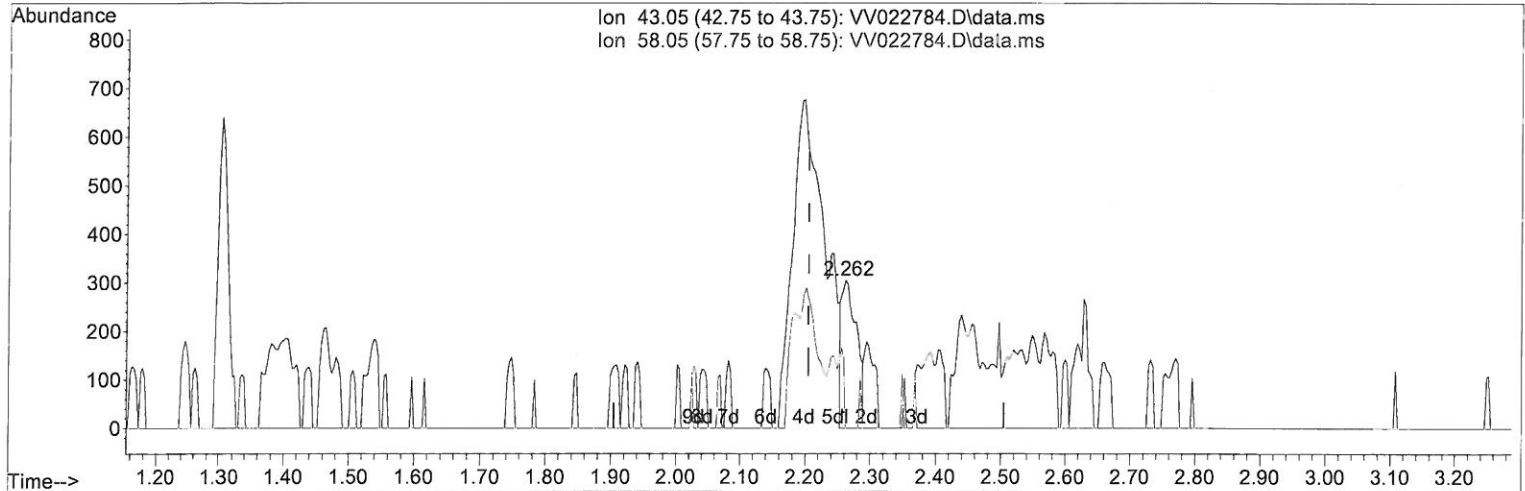

TIC: VV022784.D\data.ms

(13) Acetone (T)

2.262min (+ 0.058) 0.41 ug/L

response 492

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	17.68
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022784.D
 Acq On : 14 Oct 2021 11:55
 Operator : SY/MD
 Sample : M4167-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YATLO

Manual Integrations
 APPROVED

MMDadoda
 10/15/2021 12:02:52 PM

Quant Time: Oct 15 01:59:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 15 01:58:00 2021
 Response via : Initial Calibration

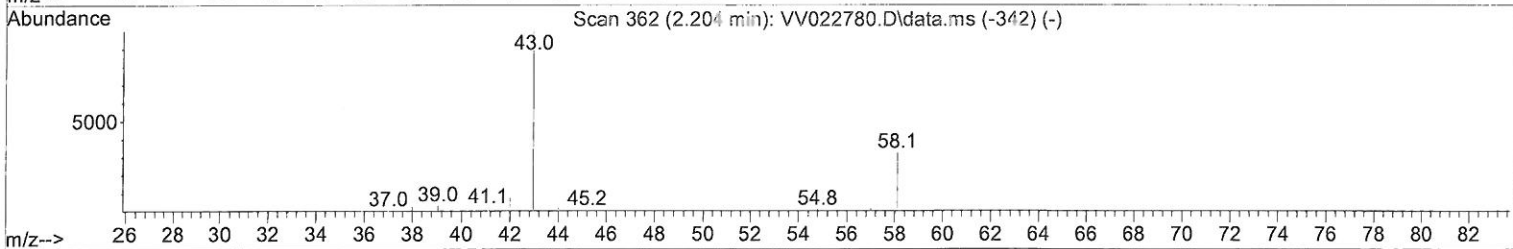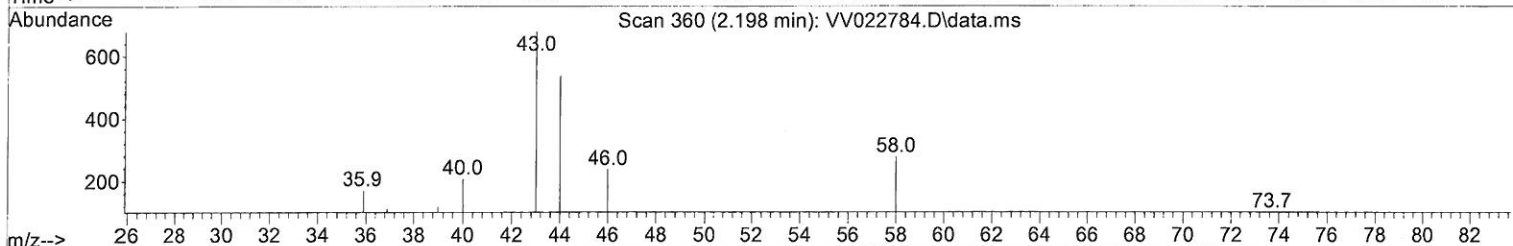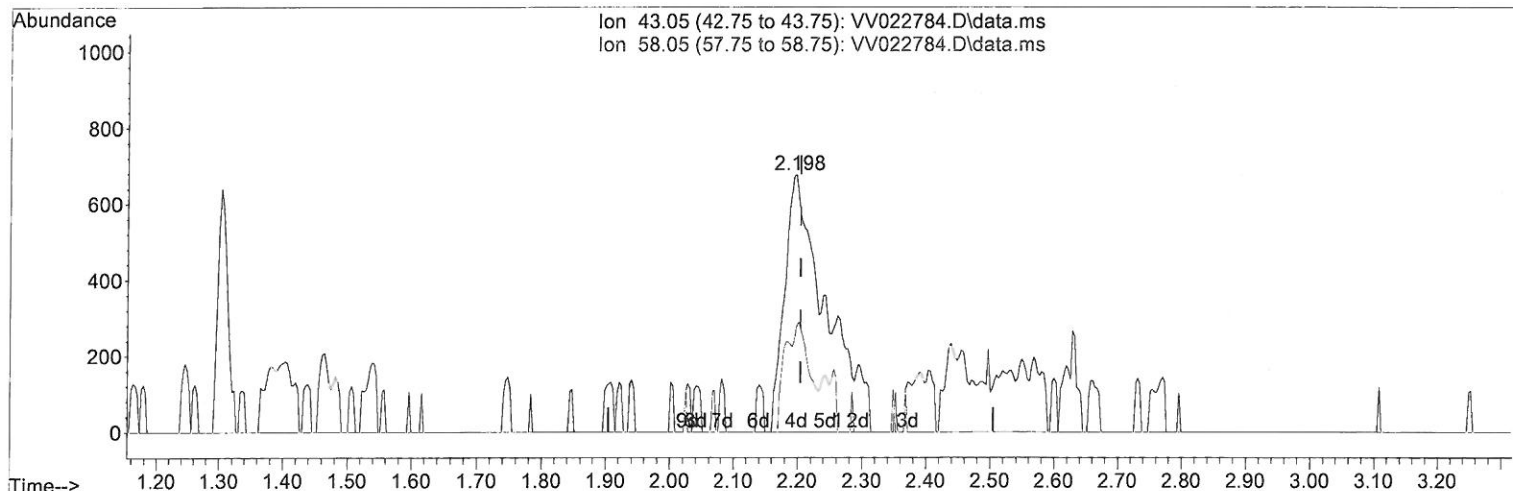

TIC: VV022784.D\data.ms

(13) Acetone (T)

2.198min (-0.006) 2.52 ug/L m

response 3012

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	2.89
0.00	0.00	0.00
0.00	0.00	0.00

7 MB
 10/22/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022784.D
 Acq On : 14 Oct 2021 11:55
 Operator : SY/MD
 Sample : M4167-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YATLO

Manual Integrations
 APPROVED

MMDadoda
 10/15/2021 12:02:52 PM

Quant Time: Oct 15 01:59:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 15 01:58:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	119053	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	121199	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55260	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	31546	3.851	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.000%	
7) Chloroethane-d5	1.568	69	31989	4.346	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	87.000%	
11) 1,1-Dichloroethene-d2	2.108	63	45482	2.831	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	56.600%#	
20) 2-Butanone-d5	3.905	46	88929	41.406	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	82.820%	
24) Chloroform-d	4.352	84	81911	4.853	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.000%	
26) 1,2-Dichloroethane-d4	5.037	65	37658	4.597	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.000%	
32) Benzene-d6	5.053	84	150624	4.175	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.400%	
36) 1,2-Dichloropropane-d6	6.072	67	49442	4.627	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	92.600%	
41) Toluene-d8	7.320	98	125875	4.036	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	80.800%	
43) trans-1,3-Dichloroprop...	7.629	79	14569	4.110	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.200%	
46) 2-Hexanone-d5	8.092	63	68876	48.218	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.440%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35999	4.973	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	99.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	53225	5.195	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.800%	
Target Compounds					Qvalue	
13) Acetone	2.198	43	3012m	2.515	ug/L	
30) Cyclohexane	4.683	56	4167	0.326	ug/L	

MD
 10/22/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed