


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022809.D
Acq On : 14 Oct 2021 22:40
Operator : SY/MD
Sample : M4223-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1




Quant Time: Oct 15 06:45:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 06:41:28 2021
Response via : Initial Calibration

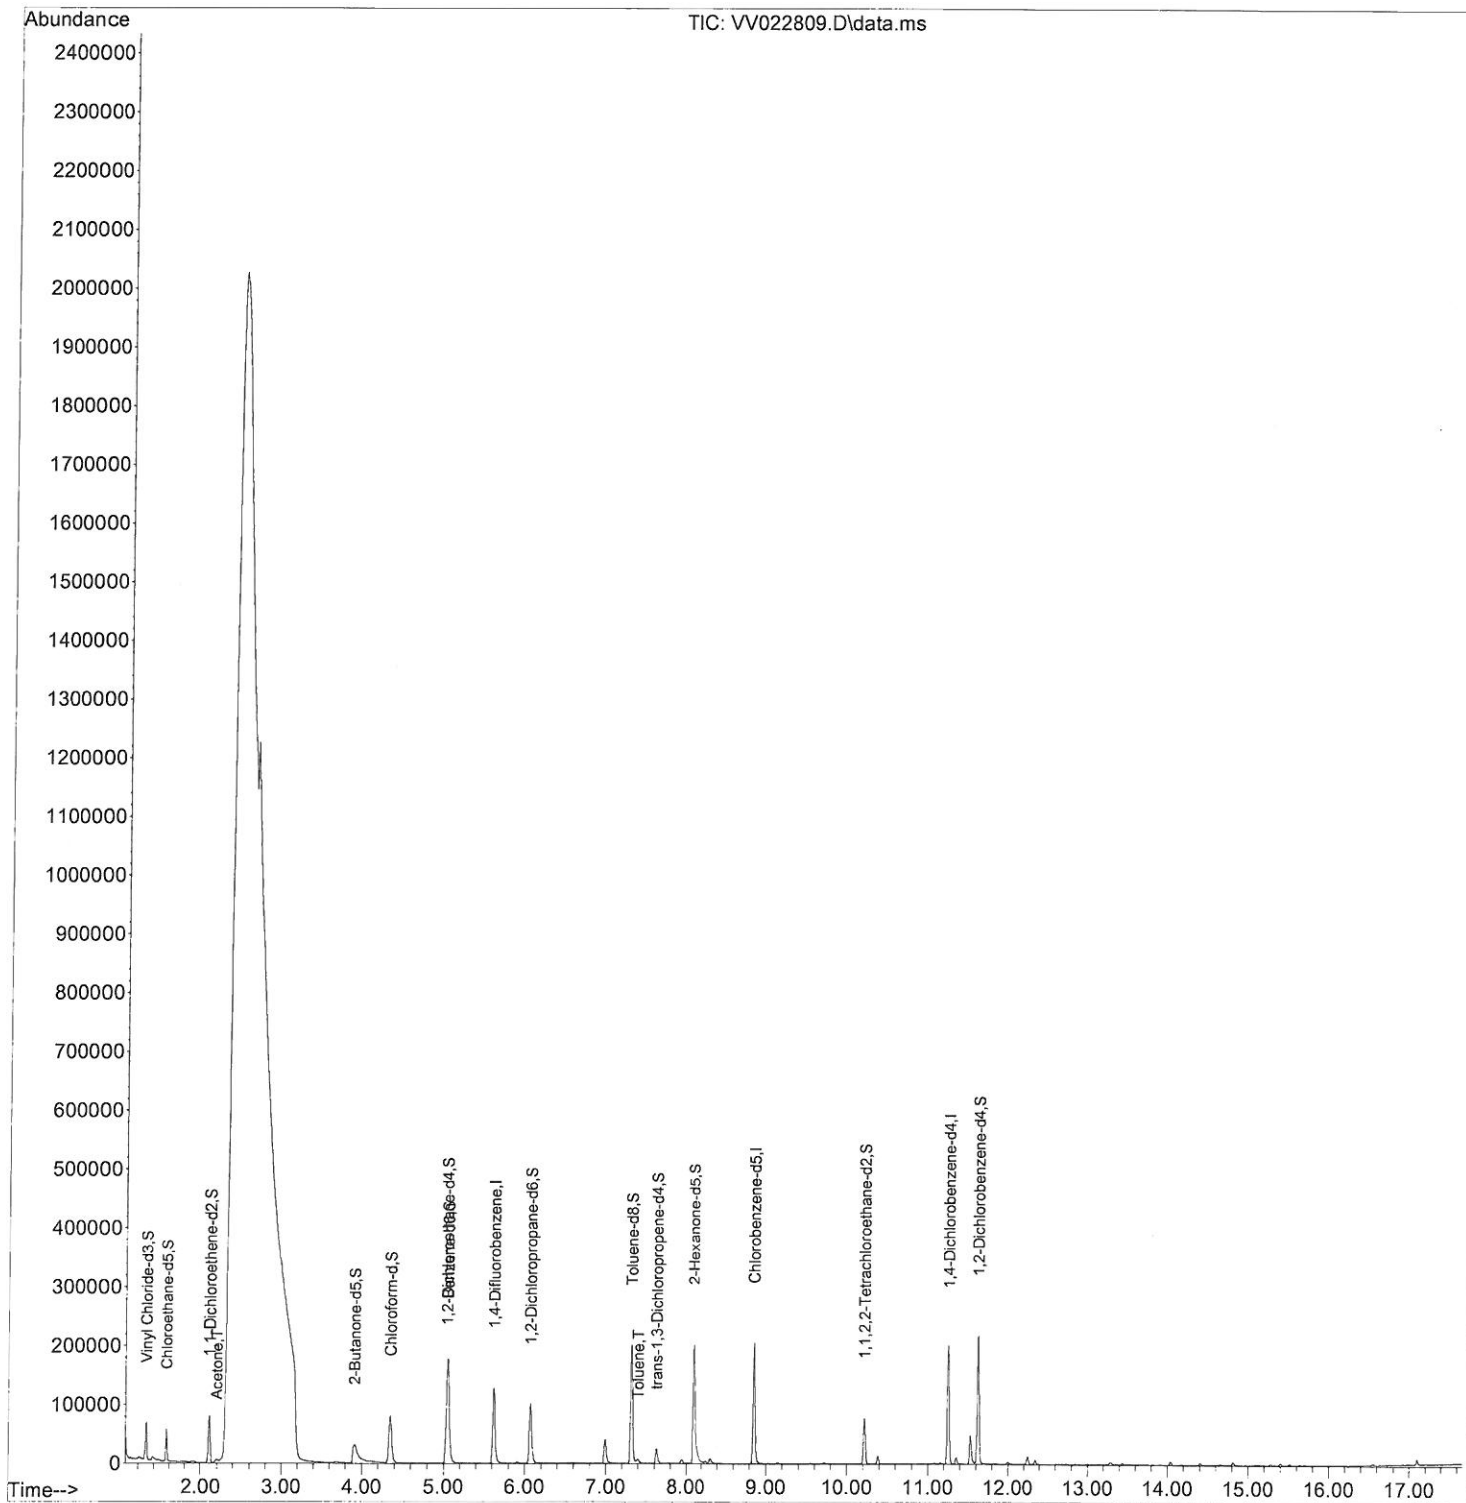

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022809.D
Acq On : 14 Oct 2021 22:40
Operator : SY/MD
Sample : M4223-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Oct 15 06:45:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 06:41:28 2021
Response via : Initial Calibration

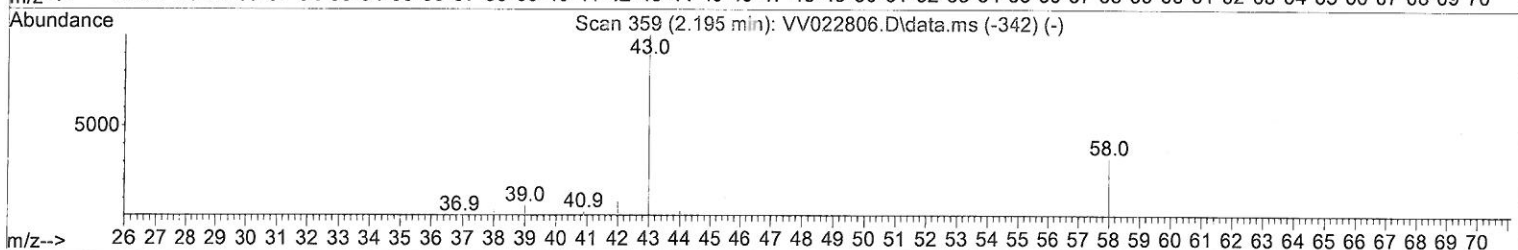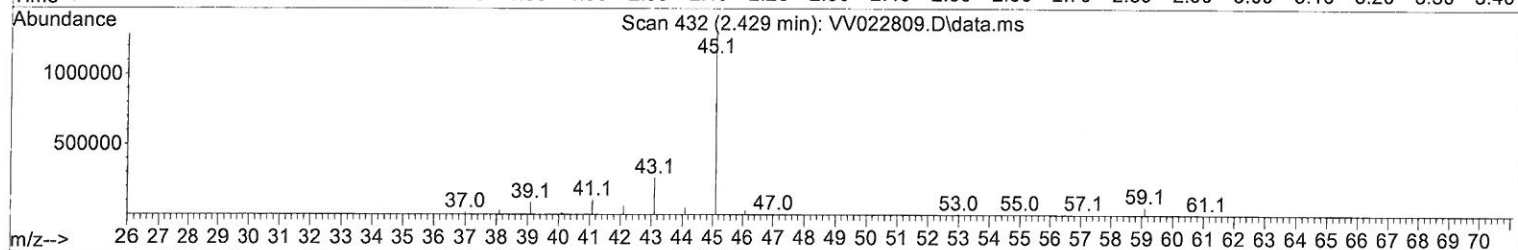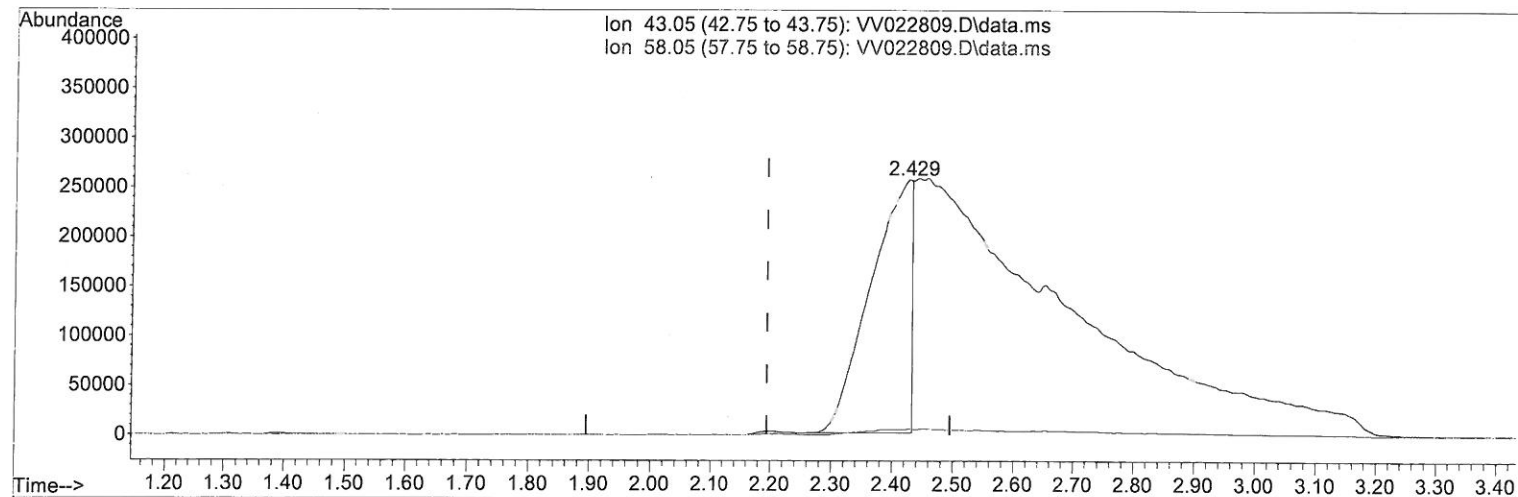

TIC: VV022809.D\data.ms

(13) Acetone (T)

2.429min (+ 0.235) 1058.83 ug/L




response 1210509

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	0.08
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022809.D
Acq On : 14 Oct 2021 22:40
Operator : SY/MD
Sample : M4223-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Oct 15 06:45:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 06:41:28 2021
Response via : Initial Calibration

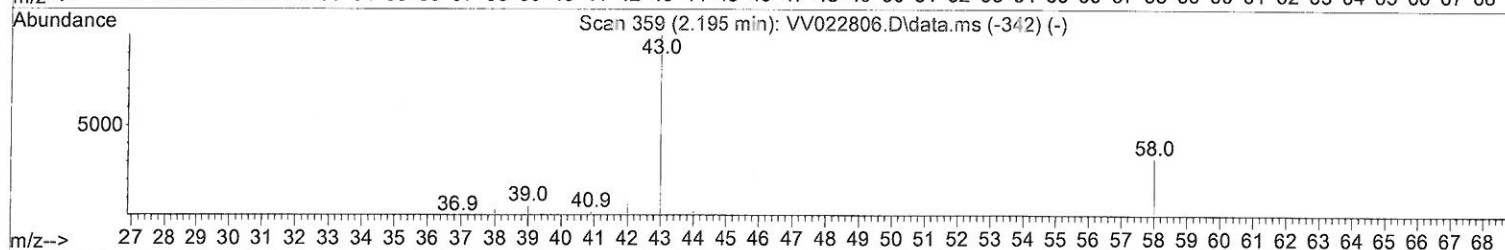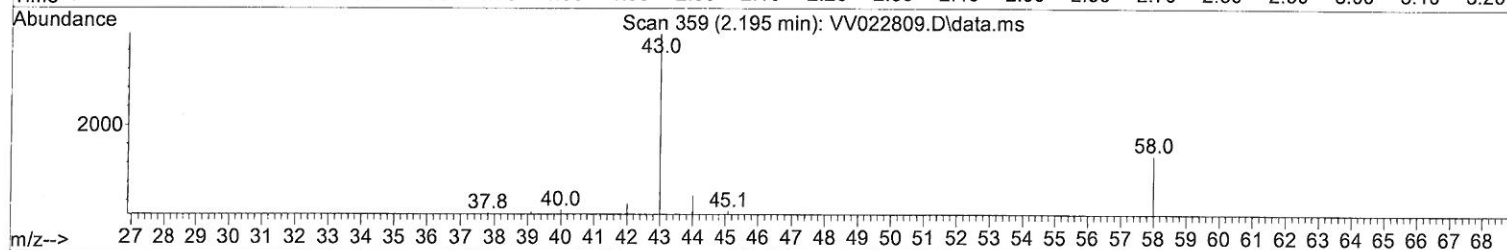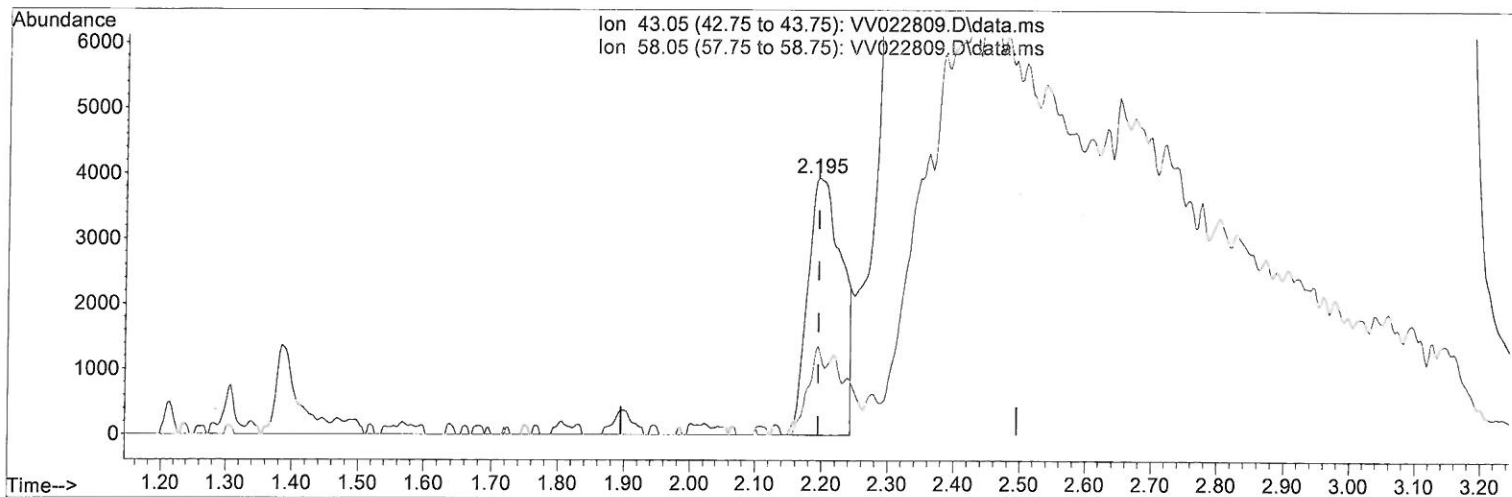

TIC: VV022809.D\data.ms

(13) Acetone (T)

2.195min (-0.000) 12.22 ug/L m

response 13976

Ion	Exp%	Act%
-----	------	------

43.05	100.00	100.00
-------	--------	--------

58.05	12.10	6.55
-------	-------	------

0.00	0.00	0.00
------	------	------

0.00	0.00	0.00
------	------	------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101421\
 Data File : VW022809.D
 Acq On : 14 Oct 2021 22:40
 Operator : SY/MD
 Sample : M4223-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Quant Time: Oct 15 06:45:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 15 06:41:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	113649	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	116811	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	55232	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	36677	4.691	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	93.800%		
7) Chloroethane-d5	1.564	69	32509	4.627	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	92.600%		
11) 1,1-Dichloroethene-d2	2.108	63	40757	2.657	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	53.200%#		
20) 2-Butanone-d5	3.908	46	80854	39.437	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	78.880%		
24) Chloroform-d	4.349	84	83203	5.164	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	103.200%		
26) 1,2-Dichloroethane-d4	5.037	65	39022	4.990	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	99.800%		
32) Benzene-d6	5.050	84	160663	4.620	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	92.400%		
36) 1,2-Dichloropropane-d6	6.069	67	51322	4.984	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	99.600%		
41) Toluene-d8	7.317	98	135531	4.509	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	90.200%		
43) trans-1,3-Dichloroprop...	7.628	79	15644	4.579	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	91.600%		
46) 2-Hexanone-d5	8.091	63	80500	58.473	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	116.940%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	36866	5.284	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	105.600%		
66) 1,2-Dichlorobenzene-d4	11.625	152	58638	5.726	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	114.600%		
Target Compounds						
13) Acetone	2.195	43	13976m	12.225	ug/L	Qvalue
42) Toluene	7.397	91	5156	0.161	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed