

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101421\
 Data File : VW022787.D
 Acq On : 14 Oct 2021 13:05
 Operator : SY/MD
 Sample : M4181-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B82

Quant Time: Oct 15 01:59:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 15 01:58:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	120024	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	122451	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	56783	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	30157	3.65	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.00%
7) Chloroethane-d5	1.568	69	28740	3.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.40%
11) 1,1-Dichloroethene-d2	2.108	63	41112	2.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	50.80%#
20) 2-Butanone-d5	3.892	46	100855	46.58	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.16%
24) Chloroform-d	4.352	84	80626	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
26) 1,2-Dichloroethane-d4	5.037	65	37869	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
32) Benzene-d6	5.053	84	147089	4.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.80%
36) 1,2-Dichloropropane-d6	6.072	67	49140	4.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.00%
41) Toluene-d8	7.320	98	122407	3.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.60%
43) trans-1,3-Dichloroprop...	7.625	79	14794	4.13	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.60%
46) 2-Hexanone-d5	8.091	63	75515	52.33	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.66%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	36745	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.40%
66) 1,2-Dichlorobenzene-d4	11.625	152	53167	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%
Target Compounds						
13) Acetone	2.185	43	4939	4.09	ug/L	Qvalue # 35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022787.D
Acq On : 14 Oct 2021 13:05
Operator : SY/MD
Sample : M4181-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B82

Quant Time: Oct 15 01:59:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 01:58:00 2021
Response via : Initial Calibration

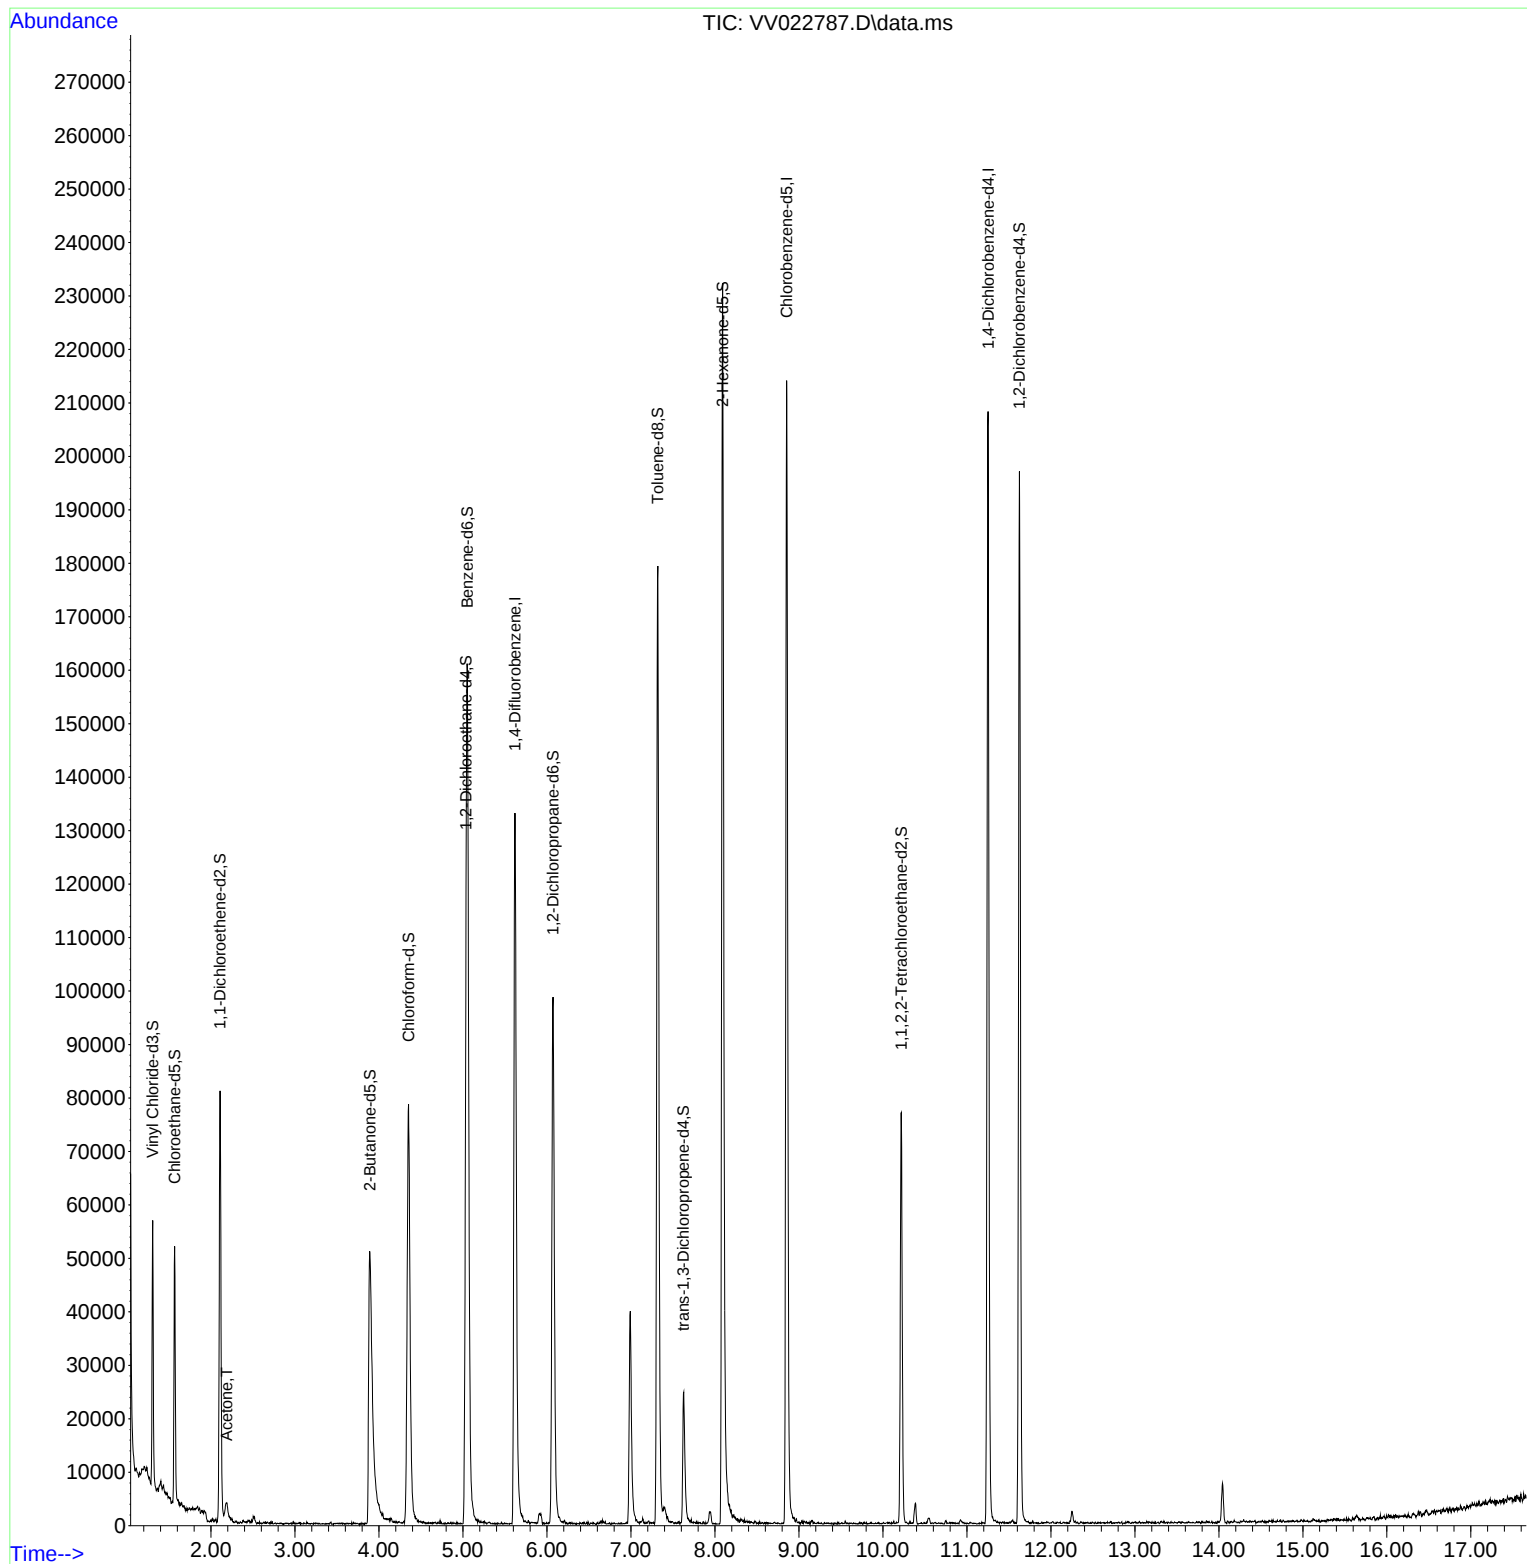

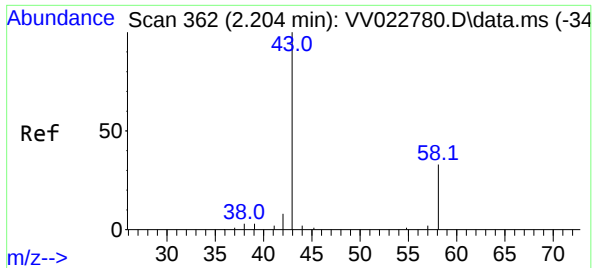

#13
 Acetone
 Concen: 4.09 ug/L
 RT: 2.185 min Scan# 356
 Delta R.T. -0.019 min
 Lab File: VV022787.D
 Acq: 14 Oct 2021 13:05

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B82

Tgt Ion: 43 Resp: 4939
 Ion Ratio Lower Upper
 43 100
 58 37.5 0.0 24.2#

