

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101421\
 Data File : VW022788.D
 Acq On : 14 Oct 2021 13:29
 Operator : SY/MD
 Sample : M4205-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B84

Quant Time: Oct 15 01:59:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 15 01:58:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	111473	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	116625	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	54962	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	27111	3.53	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.60%
7) Chloroethane-d5	1.568	69	25942	3.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.20%
11) 1,1-Dichloroethene-d2	2.108	63	37703	2.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	50.20%#
20) 2-Butanone-d5	3.889	46	102966	51.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.40%
24) Chloroform-d	4.349	84	80133	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
26) 1,2-Dichloroethane-d4	5.037	65	38117	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
32) Benzene-d6	5.053	84	145641	4.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.80%
36) 1,2-Dichloropropane-d6	6.072	67	48281	4.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.00%
41) Toluene-d8	7.317	98	117261	3.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.20%
43) trans-1,3-Dichloroprop...	7.625	79	13934	4.09	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.80%
46) 2-Hexanone-d5	8.088	63	79472	57.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	115.64%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	38354	5.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.20%
66) 1,2-Dichlorobenzene-d4	11.625	152	52541	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%
Target Compounds					Qvalue	
13) Acetone	2.179	43	5112	4.56	ug/L	# 49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022788.D
Acq On : 14 Oct 2021 13:29
Operator : SY/MD
Sample : M4205-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B84

Quant Time: Oct 15 01:59:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 01:58:00 2021
Response via : Initial Calibration

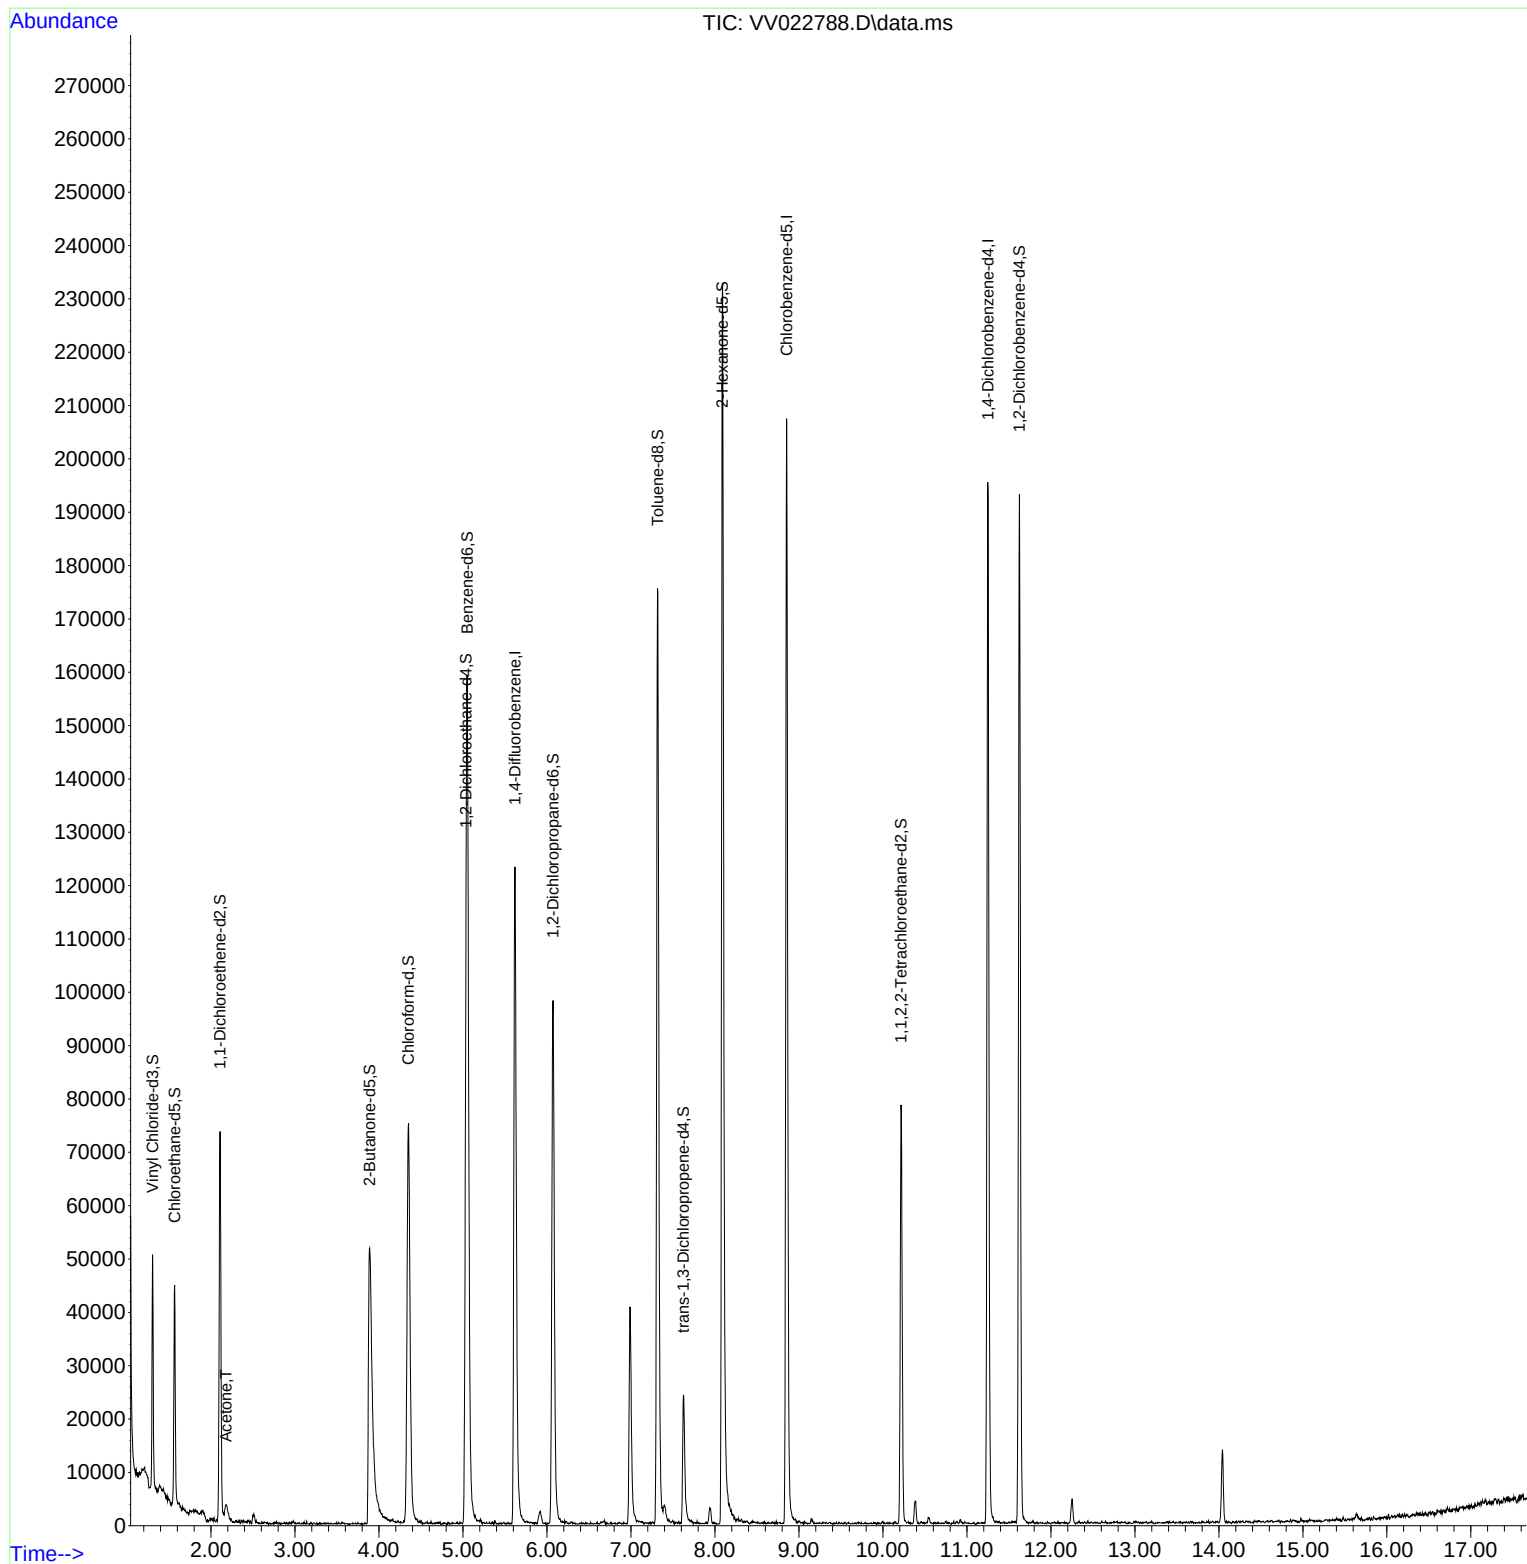

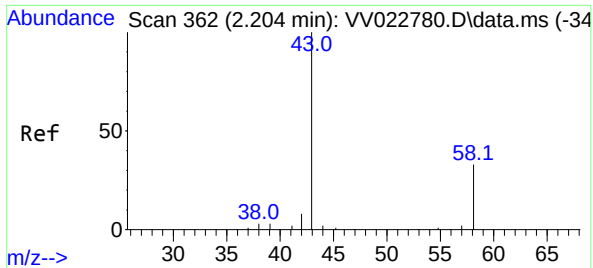

#13
 Acetone
 Concen: 4.56 ug/L
 RT: 2.179 min Scan# 354
 Delta R.T. -0.026 min
 Lab File: VV022788.D
 Acq: 14 Oct 2021 13:29

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B84

Tgt Ion: 43 Resp: 5112
 Ion Ratio Lower Upper
 43 100
 58 31.8 0.0 24.2#

