

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101421\
 Data File : VW022789.D
 Acq On : 14 Oct 2021 13:53
 Operator : SY/MD
 Sample : M4207-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B90

Quant Time: Oct 15 01:59:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 15 01:58:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	121424	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	124804	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	58630	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	31305	3.75	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.00%
7) Chloroethane-d5	1.568	69	30807	4.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.00%
11) 1,1-Dichloroethene-d2	2.108	63	43467	2.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.00%#
20) 2-Butanone-d5	3.892	46	103557	47.28	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.56%
24) Chloroform-d	4.352	84	83736	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
26) 1,2-Dichloroethane-d4	5.037	65	40378	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.053	84	154302	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.00%
36) 1,2-Dichloropropane-d6	6.072	67	50761	4.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.20%
41) Toluene-d8	7.320	98	130472	4.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.20%
43) trans-1,3-Dichloroprop...	7.625	79	16156	4.43	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.60%
46) 2-Hexanone-d5	8.091	63	80110	54.46	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.92%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39683	5.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.40%
66) 1,2-Dichlorobenzene-d4	11.625	152	55126	5.07	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.40%
Target Compounds					Qvalue	
13) Acetone	2.188	43	3426	2.80	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022789.D
Acq On : 14 Oct 2021 13:53
Operator : SY/MD
Sample : M4207-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90


Quant Time: Oct 15 01:59:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 15 01:58:00 2021
Response via : Initial Calibration

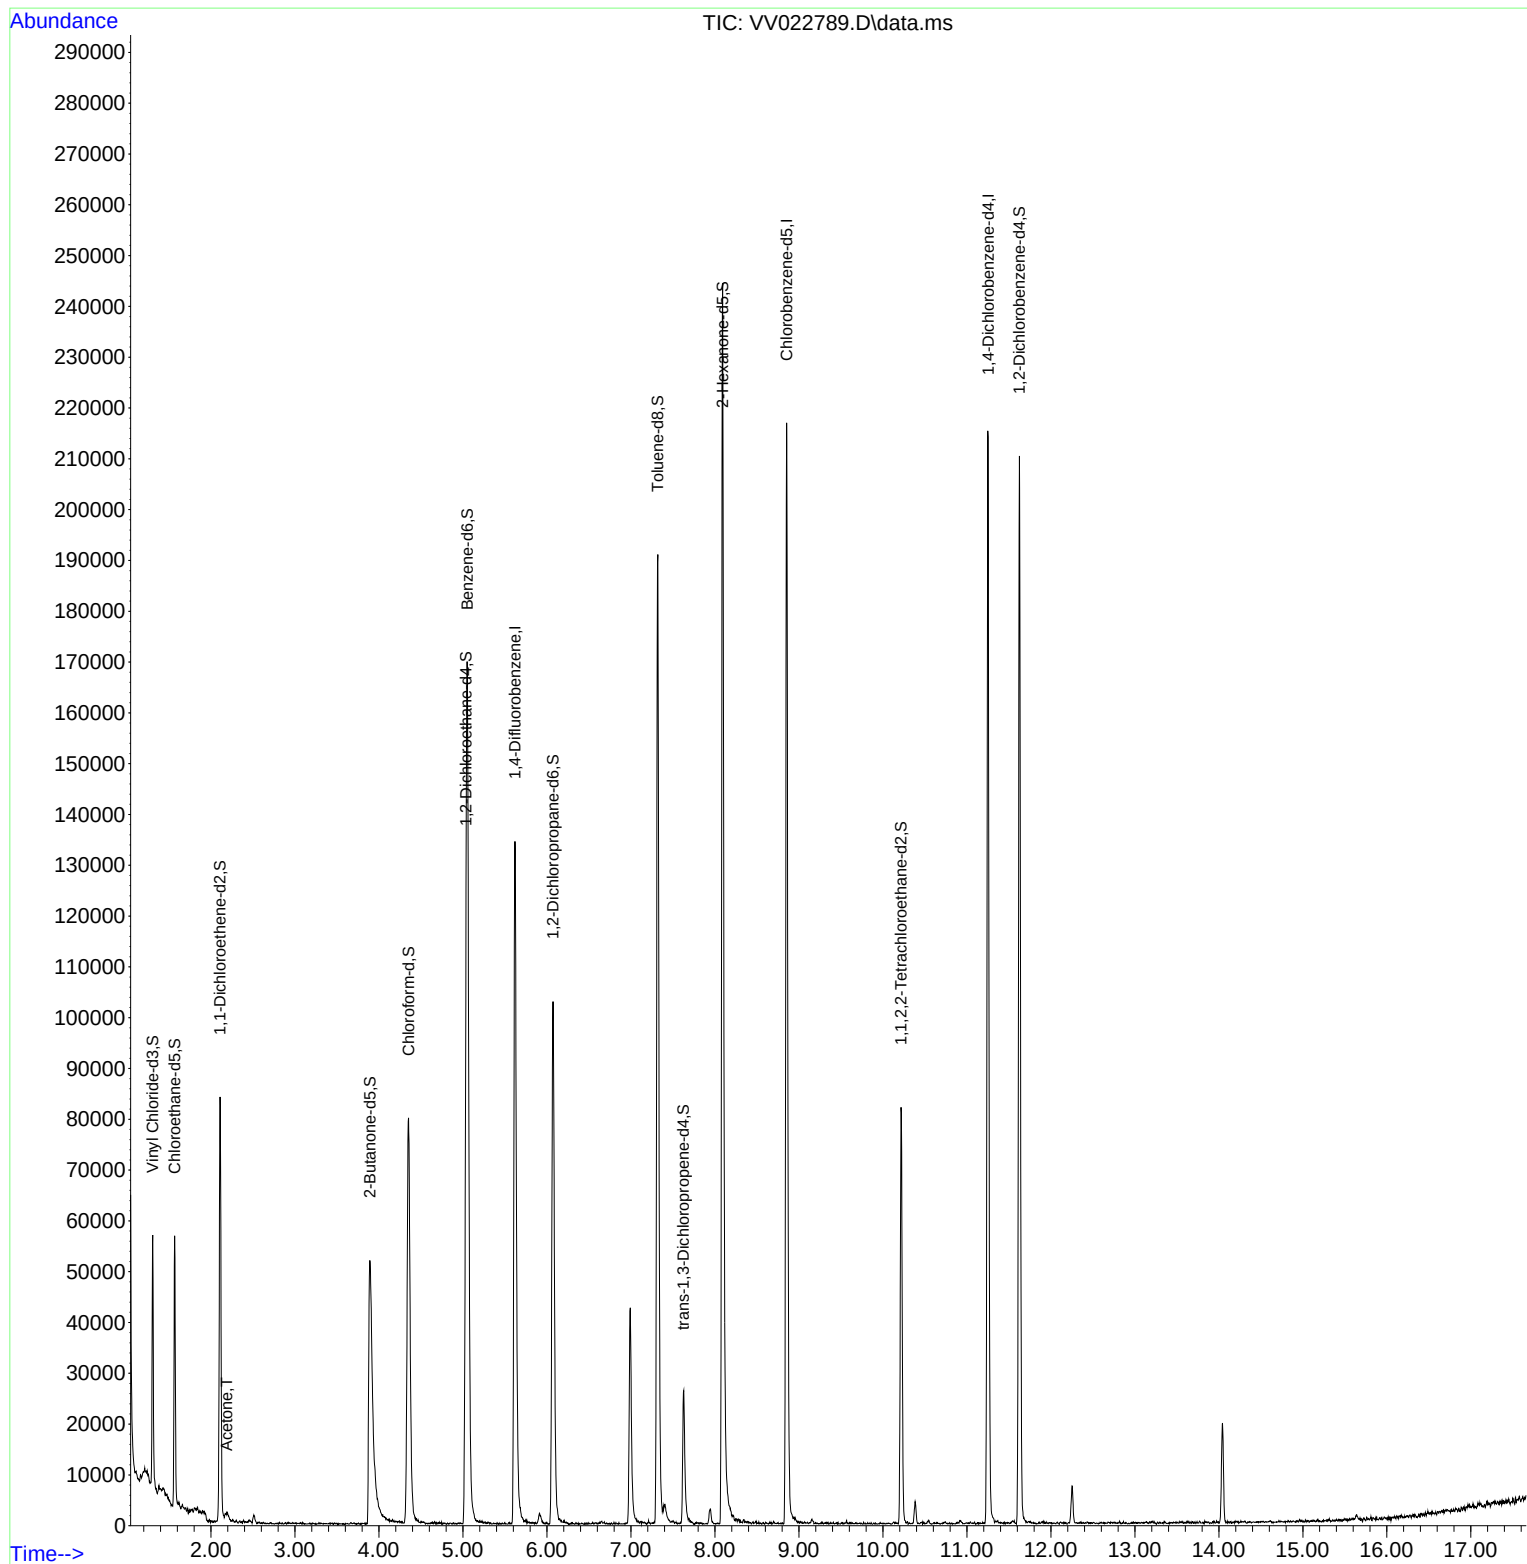

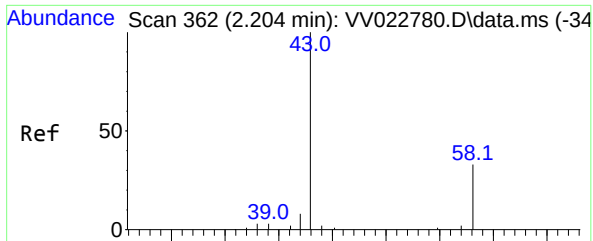

#13
Acetone
Concen: 2.80 ug/L
RT: 2.188 min Scan# 357
Delta R.T. -0.016 min
Lab File: VV022789.D
Acq: 14 Oct 2021 13:53

Instrument :
MSVOA_V
ClientSampleId :
C0B90

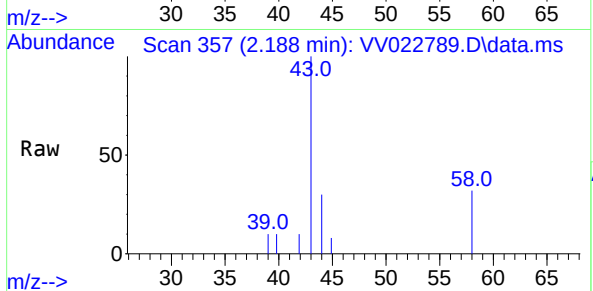

Tgt Ion: 43 Resp: 3426
Ion Ratio Lower Upper
43 100
58 19.4 0.0 24.2

