

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022782.D
 Acq On : 14 Oct 2021 11:07
 Operator : SY/MD
 Sample : M4167-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YATK7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022782.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	92	rVB	54653	55361	6.48%	1.274%
2	1.564	156	163	178	rVB	57184	65618	7.68%	1.510%
3	2.108	319	332	344	rBV	91850	135880	15.91%	3.128%
4	2.182	344	355	385	rVB	13822	42804	5.01%	0.985%
5	3.892	874	887	920	rBV	42474	147250	17.24%	3.390%
6	4.349	1010	1029	1060	rBV	77963	203044	23.78%	4.674%
7	5.047	1230	1246	1271	rBV2	163451	414363	48.52%	9.538%
8	5.616	1412	1423	1447	rBV	120064	250042	29.28%	5.756%
9	5.912	1502	1515	1546	rBV	437050	853917	100.00%	19.657%
10	6.069	1551	1564	1586	rVV	100355	202766	23.75%	4.668%
11	6.989	1838	1850	1875	rBV	39309	74715	8.75%	1.720%
12	7.317	1938	1952	1970	rBV	187012	330472	38.70%	7.607%
13	7.625	2039	2048	2071	rBV	23770	41395	4.85%	0.953%
14	7.976	2137	2157	2175	rVB2	71140	126486	14.81%	2.912%
15	8.088	2182	2192	2219	rBV	194474	362663	42.47%	8.348%
16	8.854	2412	2430	2452	rBV	197069	320853	37.57%	7.386%
17	10.217	2843	2854	2870	rBV	72435	114474	13.41%	2.635%
18	11.249	3164	3175	3197	rBV	177515	273798	32.06%	6.303%
19	11.625	3281	3292	3312	rBV	189560	301579	35.32%	6.942%
20	16.709	4866	4873	4886	rVB2	18469	26716	3.13%	0.615%




Sum of corrected areas: 4344196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022782.D
Acq On : 14 Oct 2021 11:07
Operator : SY/MD
Sample : M4167-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YATK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

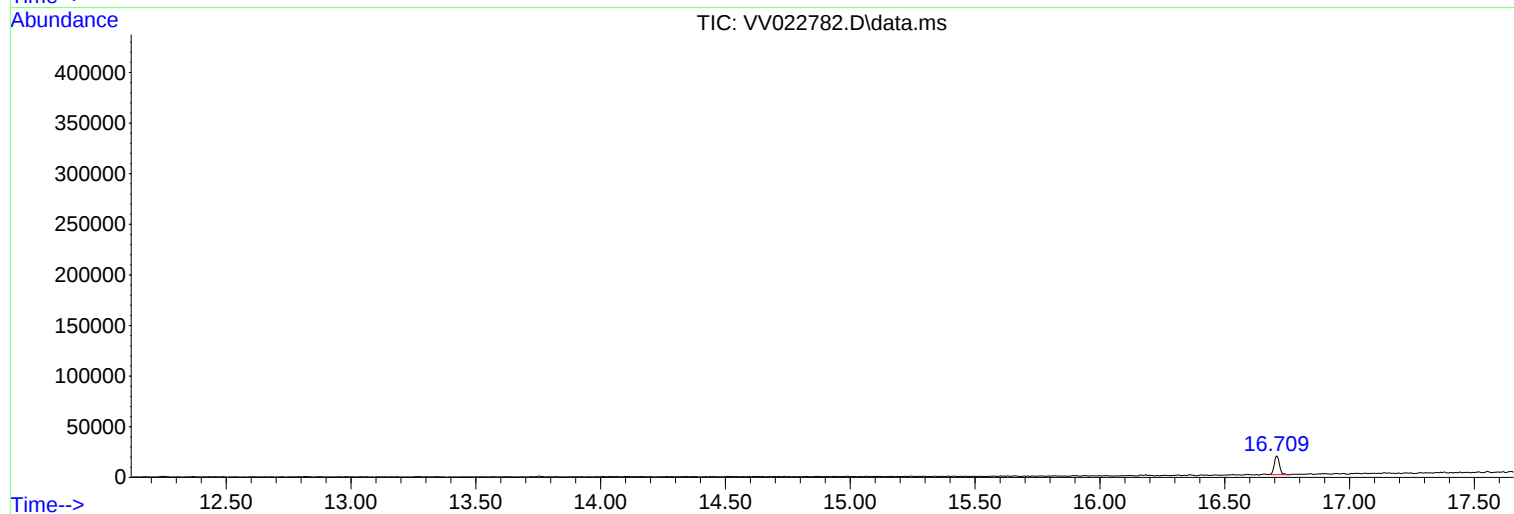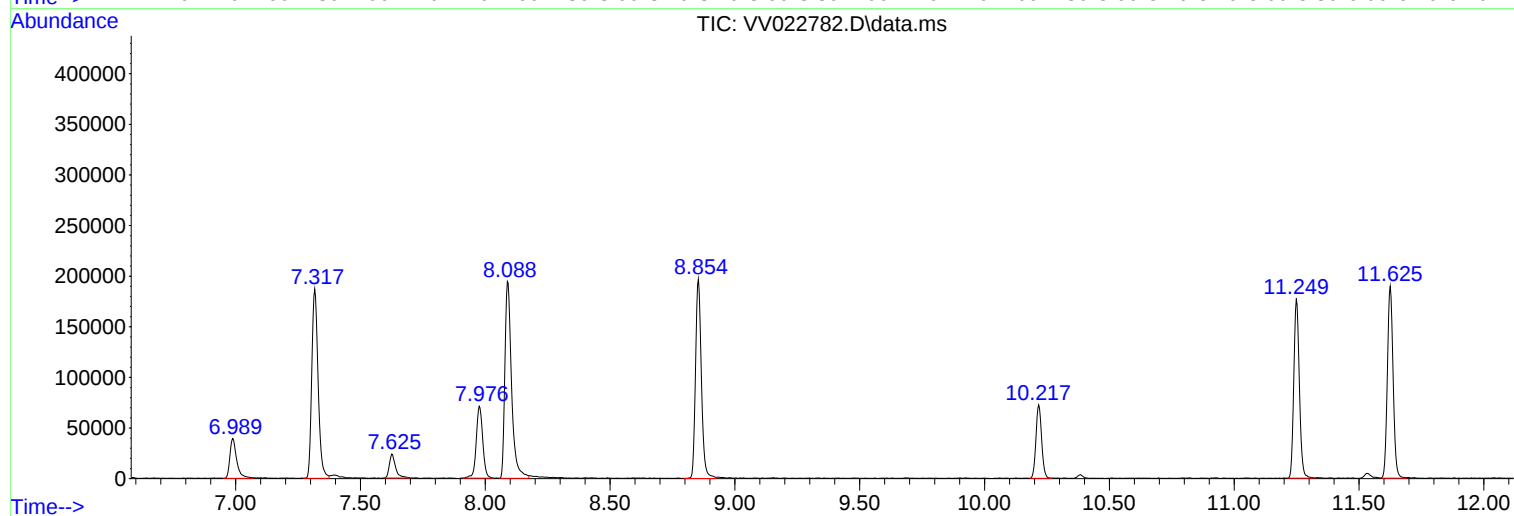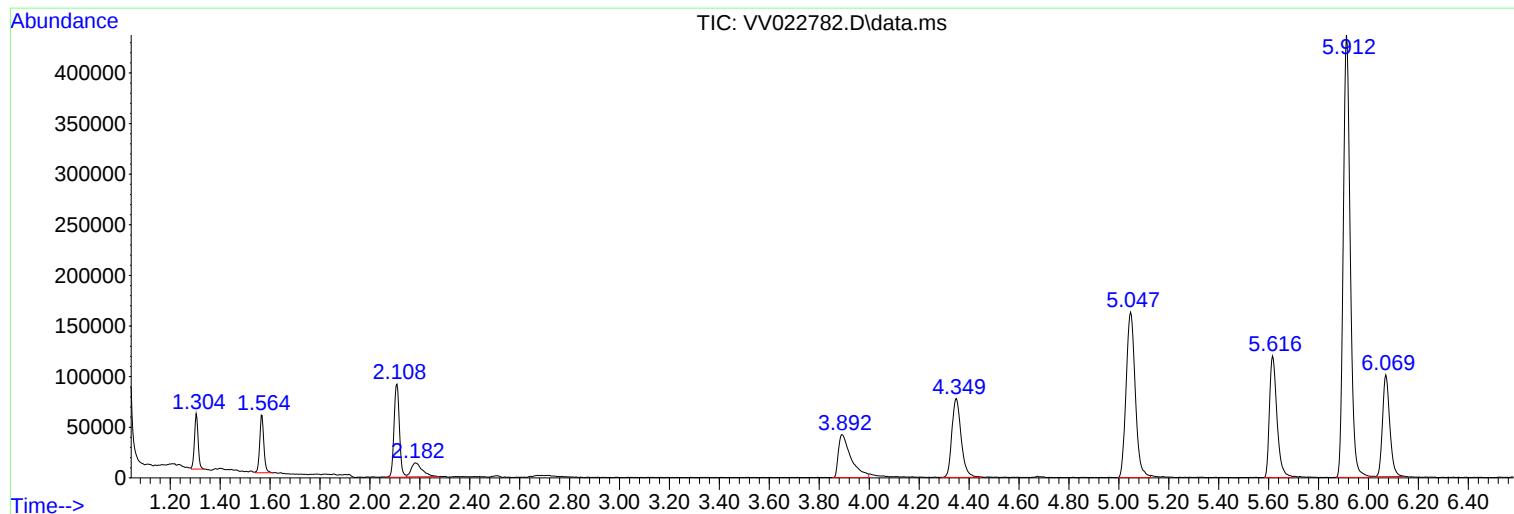

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022782.D
Acq On : 14 Oct 2021 11:07
Operator : SY/MD
Sample : M4167-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YATK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022782.D
Acq On : 14 Oct 2021 11:07
Operator : SY/MD
Sample : M4167-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YATK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
