

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022786.D
 Acq On : 14 Oct 2021 12:41
 Operator : SY/MD
 Sample : M4182-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B83

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	49565	53581	12.62%	1.540%
2	1.568	156	164	175	rBV	50617	58164	13.70%	1.672%
3	2.108	322	332	345	rBV	87060	125171	29.48%	3.598%
4	3.905	880	891	919	rBV2	38378	143814	33.87%	4.134%
5	4.352	1014	1030	1053	rBV	78518	197720	46.57%	5.683%
6	5.050	1231	1247	1275	rBV2	168293	424547	100.00%	12.203%
7	5.622	1413	1425	1446	rBV	133457	274665	64.70%	7.895%
8	6.072	1552	1565	1591	rBV2	100798	211236	49.76%	6.072%
9	6.992	1838	1851	1871	rBV2	41885	78291	18.44%	2.250%
10	7.320	1941	1953	1972	rBV	191889	339627	80.00%	9.762%
11	7.397	1972	1977	1992	rVB4	3127	6628	1.56%	0.191%
12	7.629	2040	2049	2067	rBV	25191	45692	10.76%	1.313%
13	8.092	2183	2193	2222	rBV	204758	382346	90.06%	10.990%
14	8.854	2420	2430	2455	rBV	212249	350707	82.61%	10.081%
15	10.217	2841	2854	2867	rBV	75412	119210	28.08%	3.427%
16	11.252	3164	3176	3196	rBV	210983	326054	76.80%	9.372%
17	11.535	3253	3264	3273	rBV5	6051	10540	2.48%	0.303%
18	11.625	3281	3292	3308	rBV	203173	317030	74.67%	9.113%
19	14.043	4031	4044	4057	rVB2	8975	13935	3.28%	0.401%




Sum of corrected areas: 3478958

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022786.D
Acq On : 14 Oct 2021 12:41
Operator : SY/MD
Sample : M4182-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

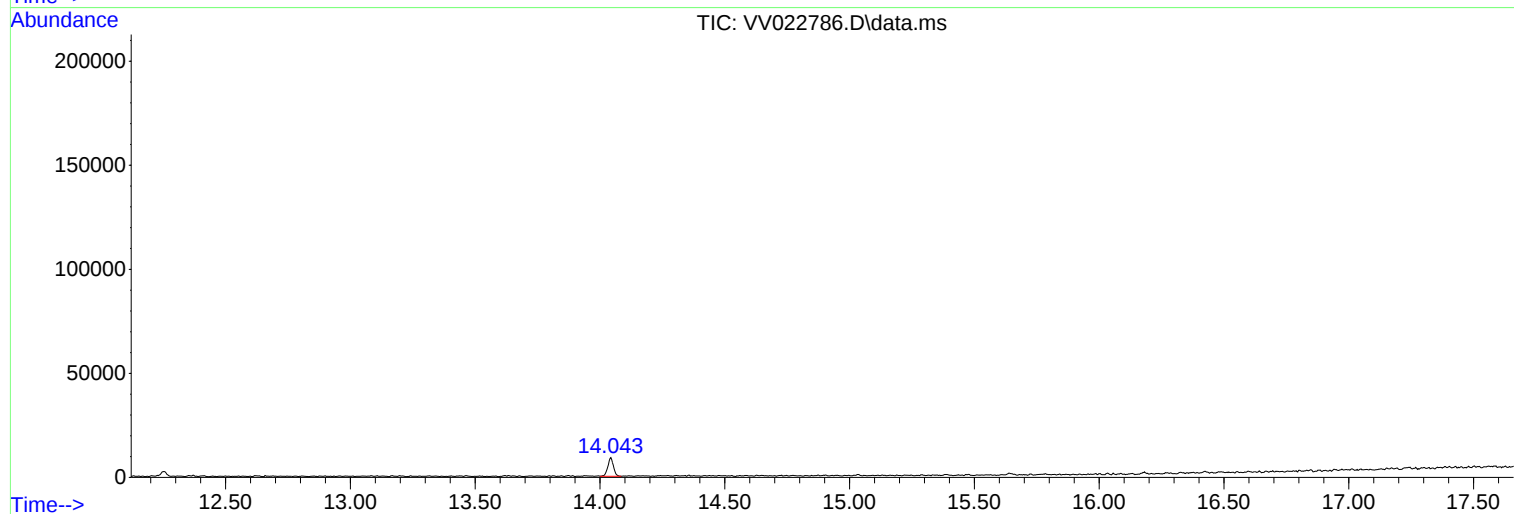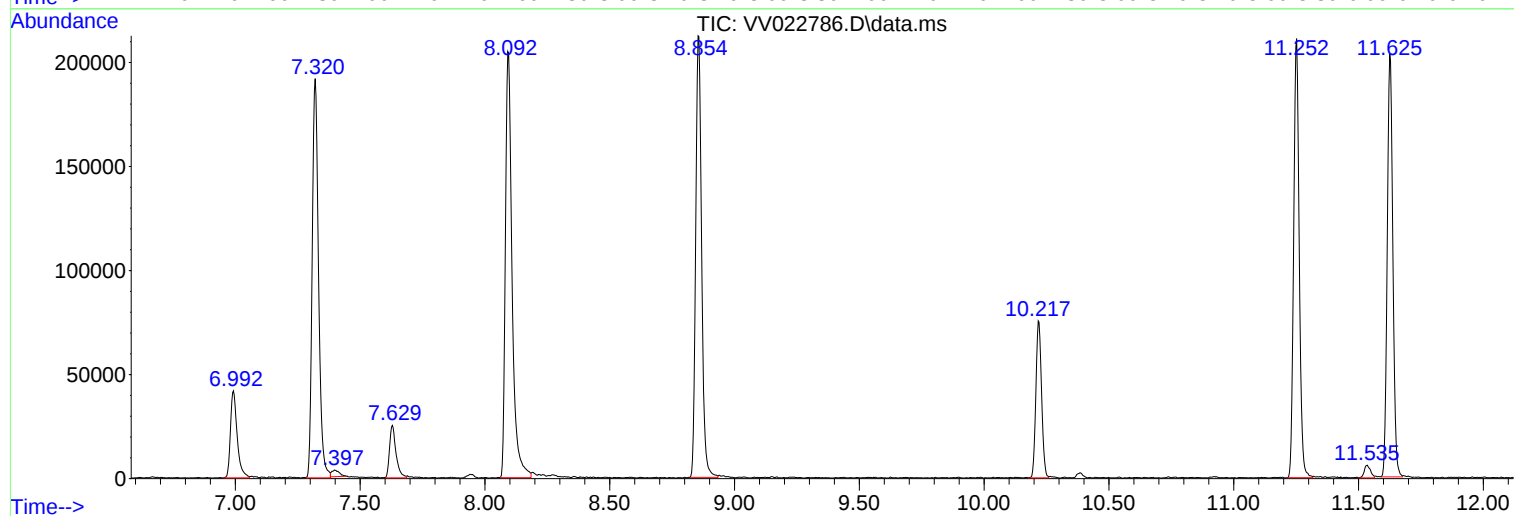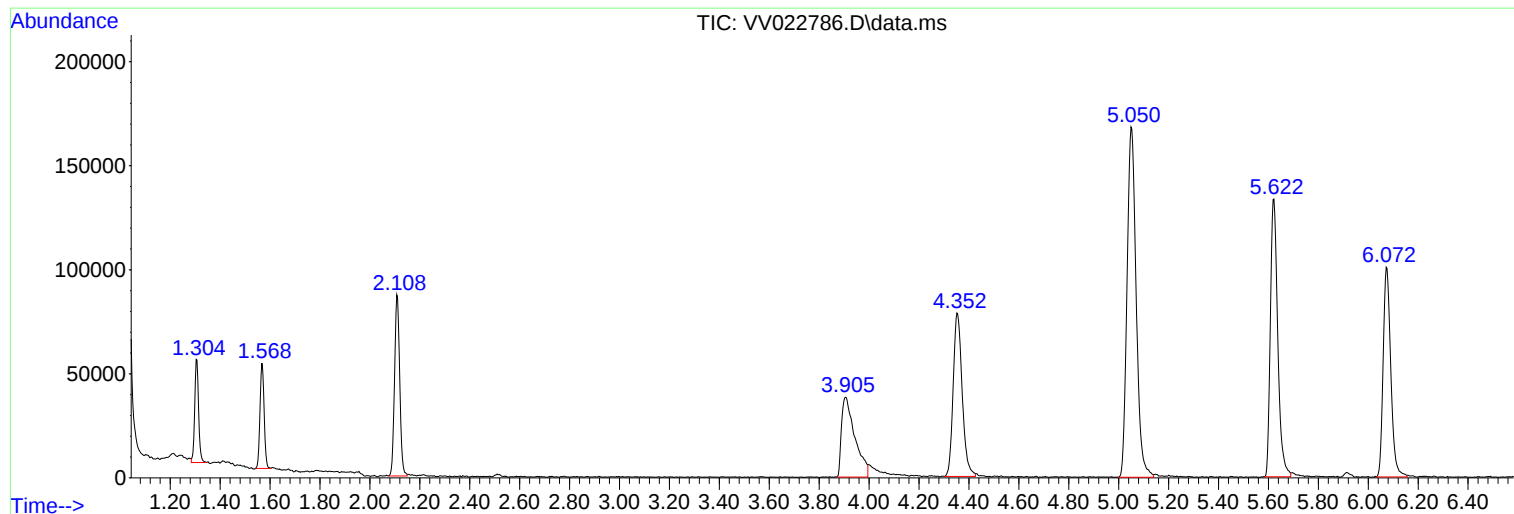

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022786.D
Acq On : 14 Oct 2021 12:41
Operator : SY/MD
Sample : M4182-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022786.D
Acq On : 14 Oct 2021 12:41
Operator : SY/MD
Sample : M4182-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
