

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022788.D
 Acq On : 14 Oct 2021 13:29
 Operator : SY/MD
 Sample : M4205-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B84

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rVB	43899	44923	10.70%	1.325%
2	1.568	156	164	176	rVB	40980	48244	11.49%	1.423%
3	2.108	322	332	344	rBV	73116	107010	25.48%	3.157%
4	2.179	347	354	371	rVB3	2956	7531	1.79%	0.222%
5	3.889	875	886	915	rBV	51644	166548	39.65%	4.914%
6	4.352	1014	1030	1056	rBV2	74721	187807	44.71%	5.541%
7	5.050	1229	1247	1274	rBV3	159149	403612	96.09%	11.908%
8	5.619	1412	1424	1447	rBV	123178	255626	60.86%	7.542%
9	5.921	1506	1518	1527	rBV10	2363	5330	1.27%	0.157%
10	6.072	1550	1565	1588	rBV2	98104	203311	48.40%	5.998%
11	6.989	1839	1850	1866	rBV	40745	76202	18.14%	2.248%
12	7.317	1940	1952	1968	rBV	175366	307946	73.32%	9.085%
13	7.625	2040	2048	2066	rBV	24076	44336	10.56%	1.308%
14	7.941	2136	2146	2156	rBV3	3037	5497	1.31%	0.162%
15	8.092	2182	2193	2217	rBV	232501	420026	100.00%	12.392%
16	8.854	2419	2430	2456	rBV	207087	335012	79.76%	9.884%
17	10.217	2840	2854	2867	rBV	78568	124364	29.61%	3.669%
18	10.384	2895	2906	2918	rBV4	4277	7240	1.72%	0.214%
19	11.249	3164	3175	3192	rBV	195195	307530	73.22%	9.073%
20	11.625	3280	3292	3307	rBV	192896	302851	72.10%	8.935%
21	12.252	3478	3487	3497	rVB2	4515	7071	1.68%	0.209%
22	14.043	4032	4044	4055	rVB2	13681	21533	5.13%	0.635%


Sum of corrected areas: 3389550

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022788.D
Acq On : 14 Oct 2021 13:29
Operator : SY/MD
Sample : M4205-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

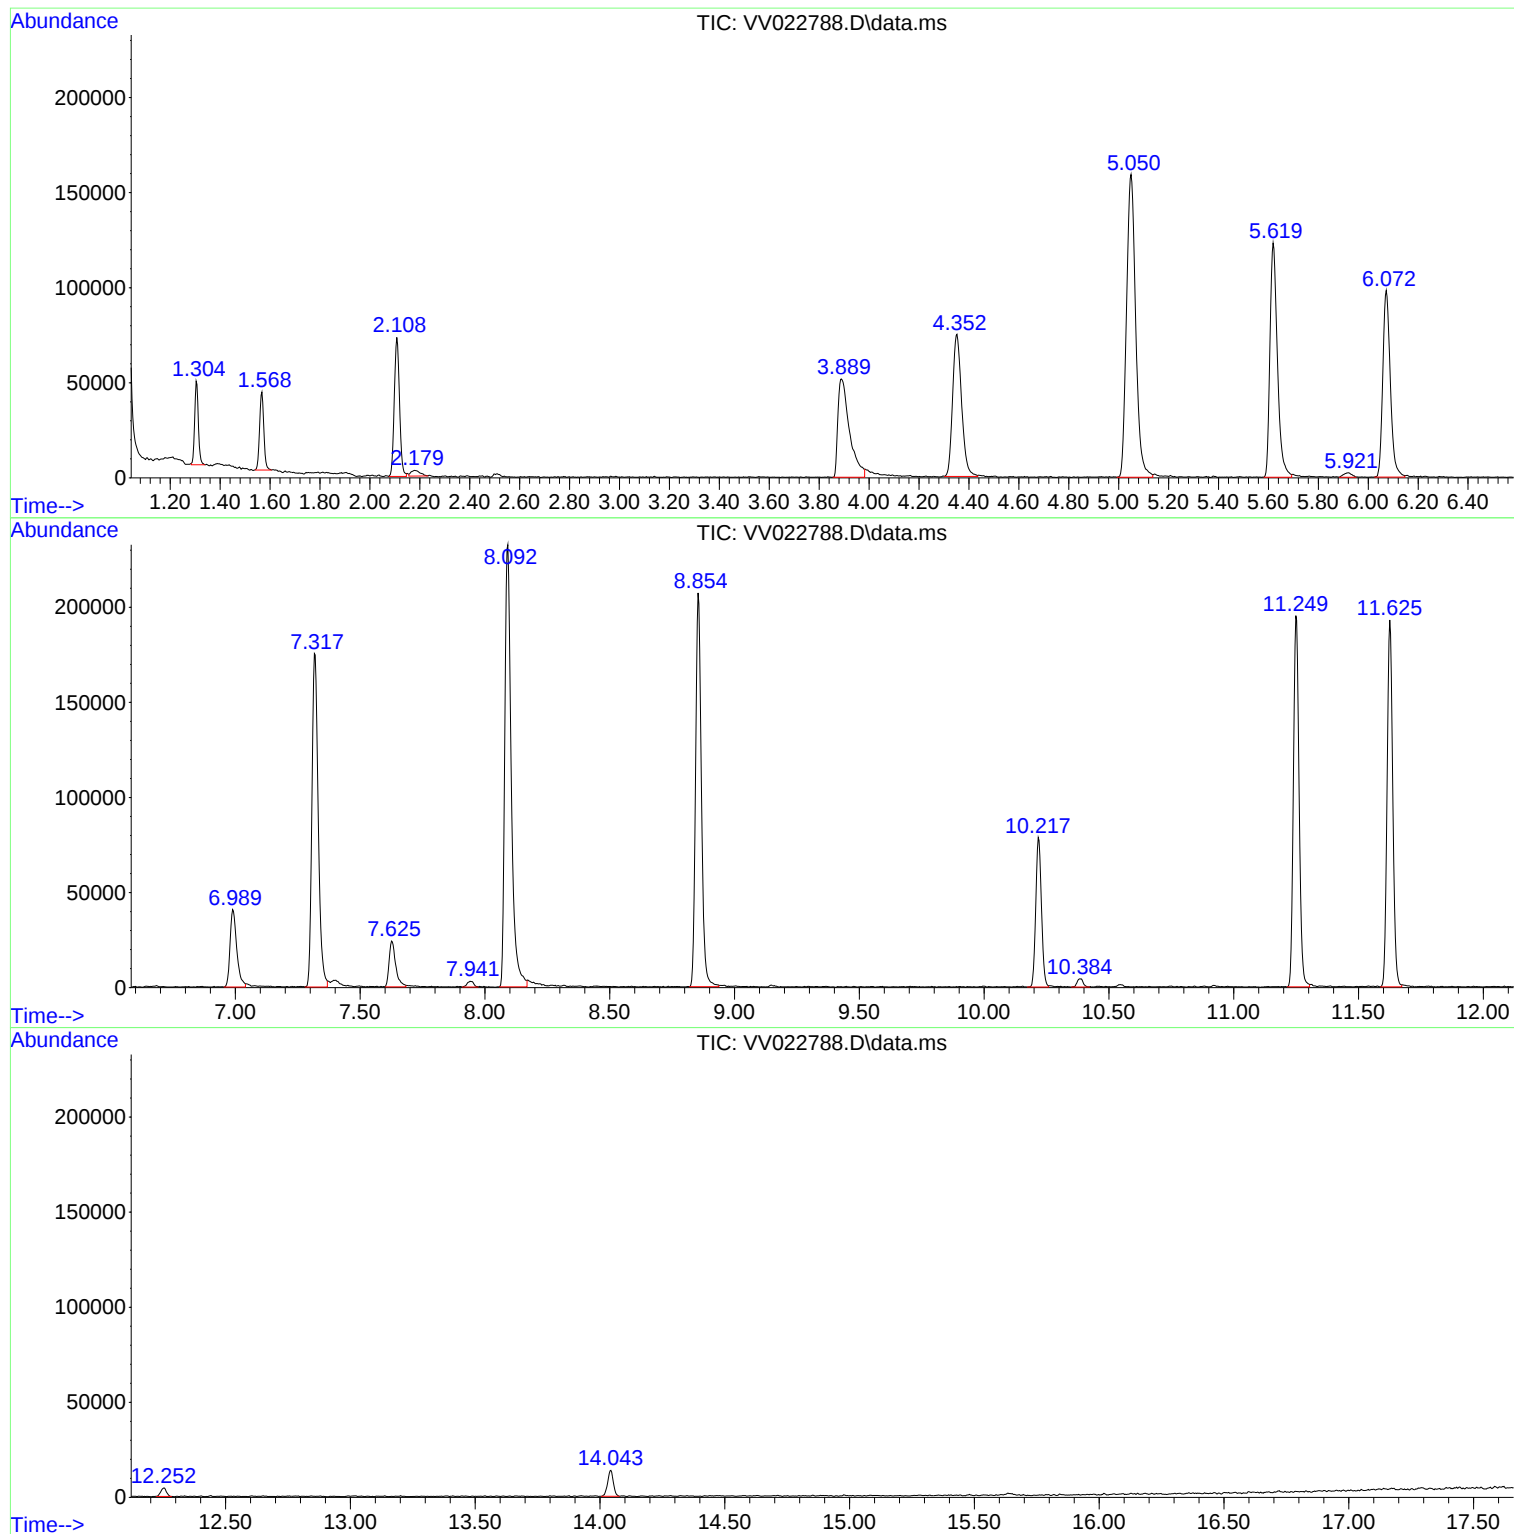

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022788.D
Acq On : 14 Oct 2021 13:29
Operator : SY/MD
Sample : M4205-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022788.D
Acq On : 14 Oct 2021 13:29
Operator : SY/MD
Sample : M4205-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
