

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022793.D
 Acq On : 14 Oct 2021 15:29
 Operator : SY/MD
 Sample : M4214-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JDGC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022793.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	92	rVB	48302	47507	12.06%	1.455%
2	1.568	156	164	175	rBV	45677	50478	12.82%	1.546%
3	2.108	321	332	345	rBV2	78677	112737	28.62%	3.453%
4	2.510	448	457	467	rVB4	4819	7953	2.02%	0.244%
5	3.915	881	894	931	rBV	30587	140548	35.69%	4.305%
6	4.352	1015	1030	1062	rVB2	74428	187195	47.53%	5.734%
7	5.050	1231	1247	1275	rBV3	157359	393846	100.00%	12.064%
8	5.619	1413	1424	1446	rBV	127834	259768	65.96%	7.957%
9	6.072	1552	1565	1585	rBV	94412	198659	50.44%	6.085%
10	6.992	1839	1851	1876	rBV	38425	74642	18.95%	2.286%
11	7.320	1941	1953	1970	rBV	172056	306937	77.93%	9.402%
12	7.625	2039	2048	2067	rBV2	22523	42154	10.70%	1.291%
13	7.940	2136	2146	2157	rVB3	3281	5550	1.41%	0.170%
14	8.095	2183	2194	2230	rBV	187219	373358	94.80%	11.436%
15	8.854	2418	2430	2451	rBV	201730	332255	84.36%	10.177%
16	10.217	2843	2854	2870	rBV	71499	115055	29.21%	3.524%
17	10.384	2896	2906	2916	rBV2	4450	6863	1.74%	0.210%
18	11.249	3164	3175	3200	rBV	193759	314239	79.79%	9.625%
19	11.625	3281	3292	3311	rBV	191373	294947	74.89%	9.034%




Sum of corrected areas: 3264691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022793.D
Acq On : 14 Oct 2021 15:29
Operator : SY/MD
Sample : M4214-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

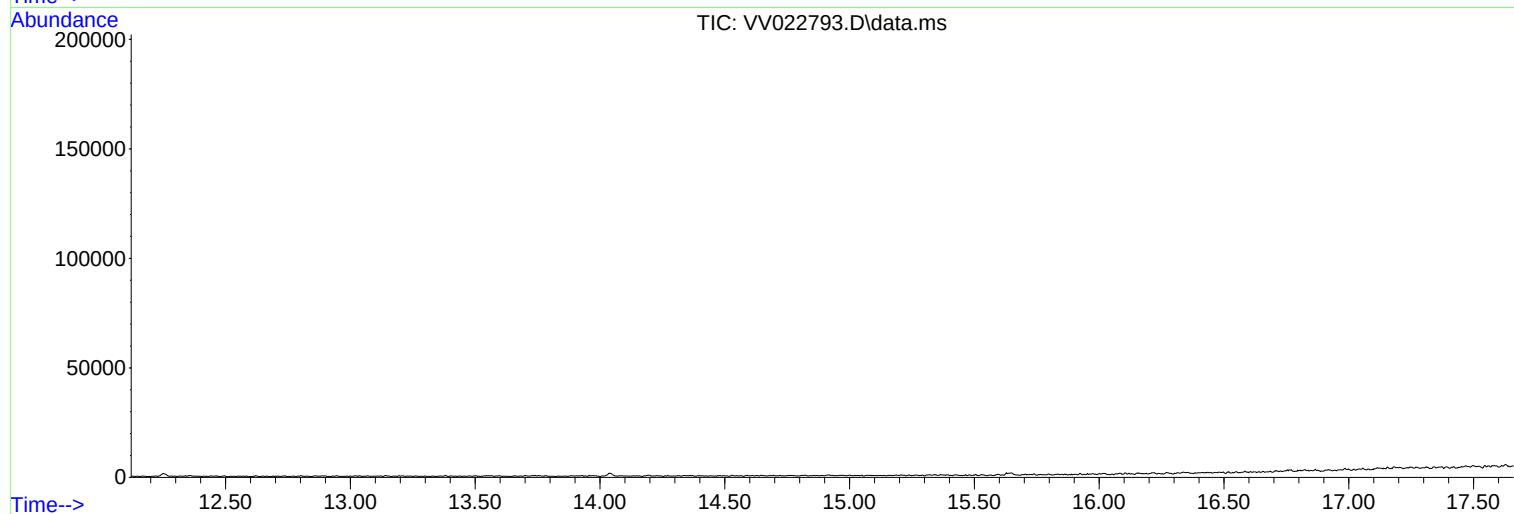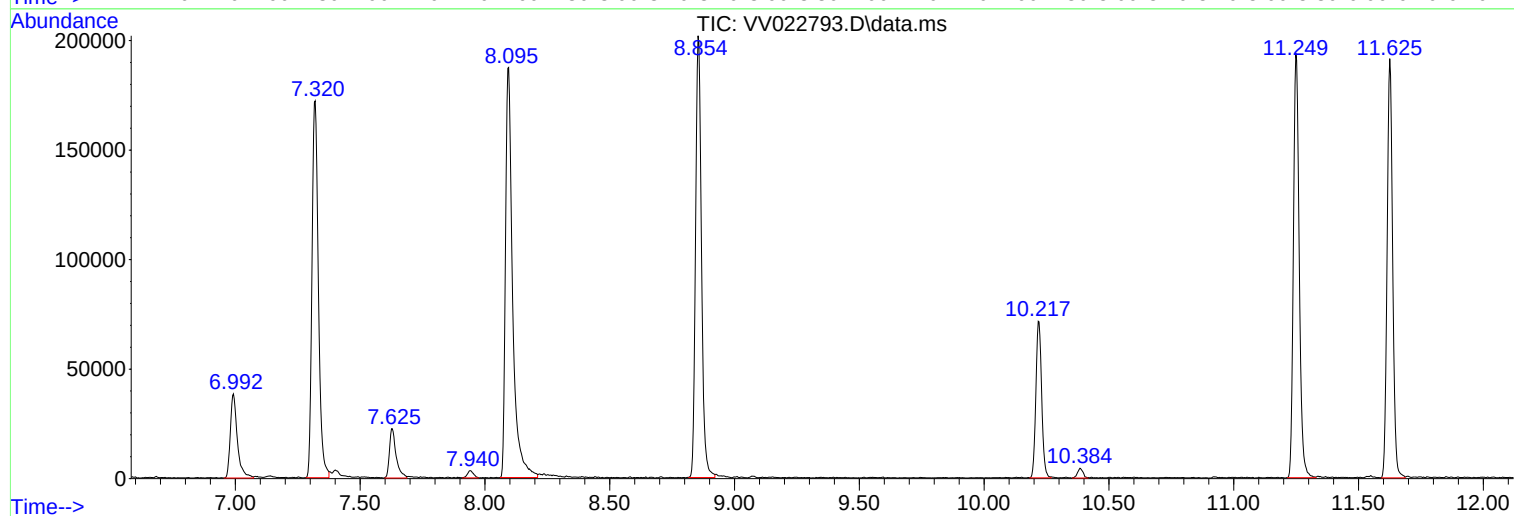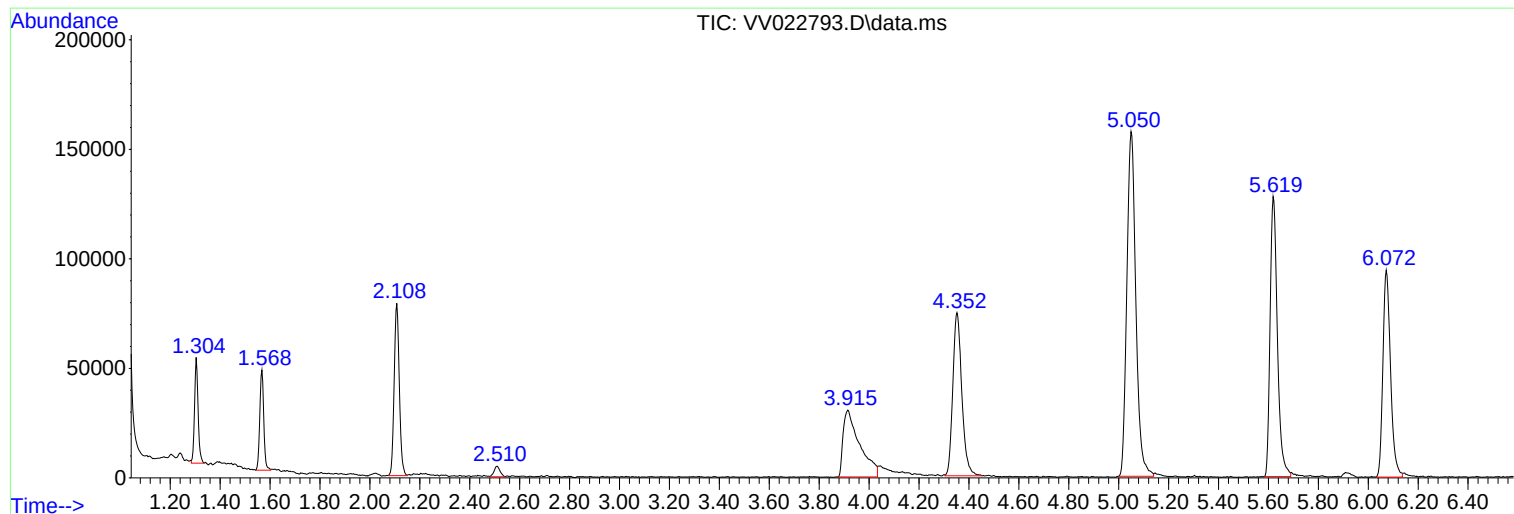

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022793.D
Acq On : 14 Oct 2021 15:29
Operator : SY/MD
Sample : M4214-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022793.D
Acq On : 14 Oct 2021 15:29
Operator : SY/MD
Sample : M4214-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
