

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022800.D
 Acq On : 14 Oct 2021 18:16
 Operator : SY/MD
 Sample : M4214-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JDGG4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	45353	46749	12.10%	1.468%
2	1.564	156	163	178	rVB	52412	60885	15.75%	1.912%
3	2.105	320	331	344	rBV	62231	89775	23.23%	2.820%
4	3.908	881	892	925	rBV2	32318	129304	33.46%	4.061%
5	4.352	1012	1030	1053	rBV2	70923	178899	46.29%	5.619%
6	5.050	1231	1247	1275	rBV3	153300	386467	100.00%	12.139%
7	5.619	1413	1424	1450	rBV	127358	259761	67.21%	8.159%
8	6.072	1552	1565	1588	rBV	93767	196334	50.80%	6.167%
9	6.992	1840	1851	1874	rBV	36139	71773	18.57%	2.254%
10	7.320	1940	1953	1972	rBV	167396	297504	76.98%	9.345%
11	7.397	1975	1977	1991	rVB7	2710	4548	1.18%	0.143%
12	7.628	2036	2049	2066	rBV	22758	42406	10.97%	1.332%
13	7.940	2139	2146	2156	rVB3	2614	4736	1.23%	0.149%
14	8.091	2183	2193	2214	rBV	198043	383647	99.27%	12.050%
15	8.853	2419	2430	2448	rBV	198812	328860	85.09%	10.329%
16	10.220	2844	2855	2872	rBV2	74923	122188	31.62%	3.838%
17	10.384	2898	2906	2915	rVB4	3715	5002	1.29%	0.157%
18	11.252	3164	3176	3199	rBV	187231	295125	76.36%	9.270%
19	11.625	3280	3292	3308	rBV	178672	279750	72.39%	8.787%




Sum of corrected areas: 3183713

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022800.D
Acq On : 14 Oct 2021 18:16
Operator : SY/MD
Sample : M4214-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

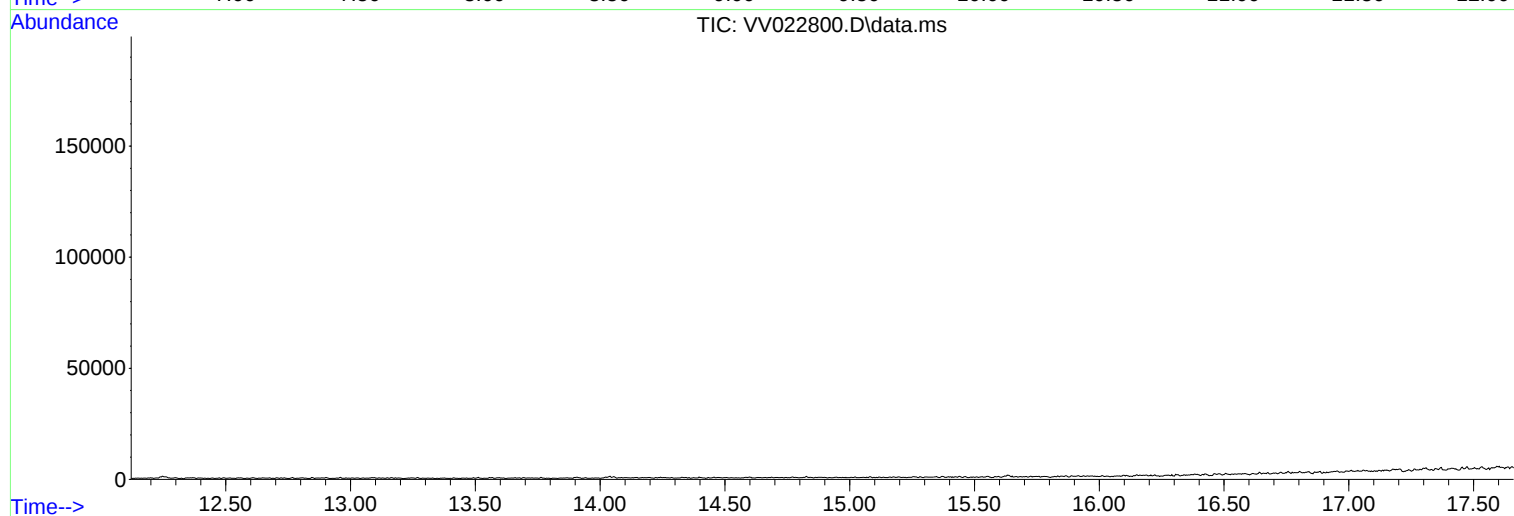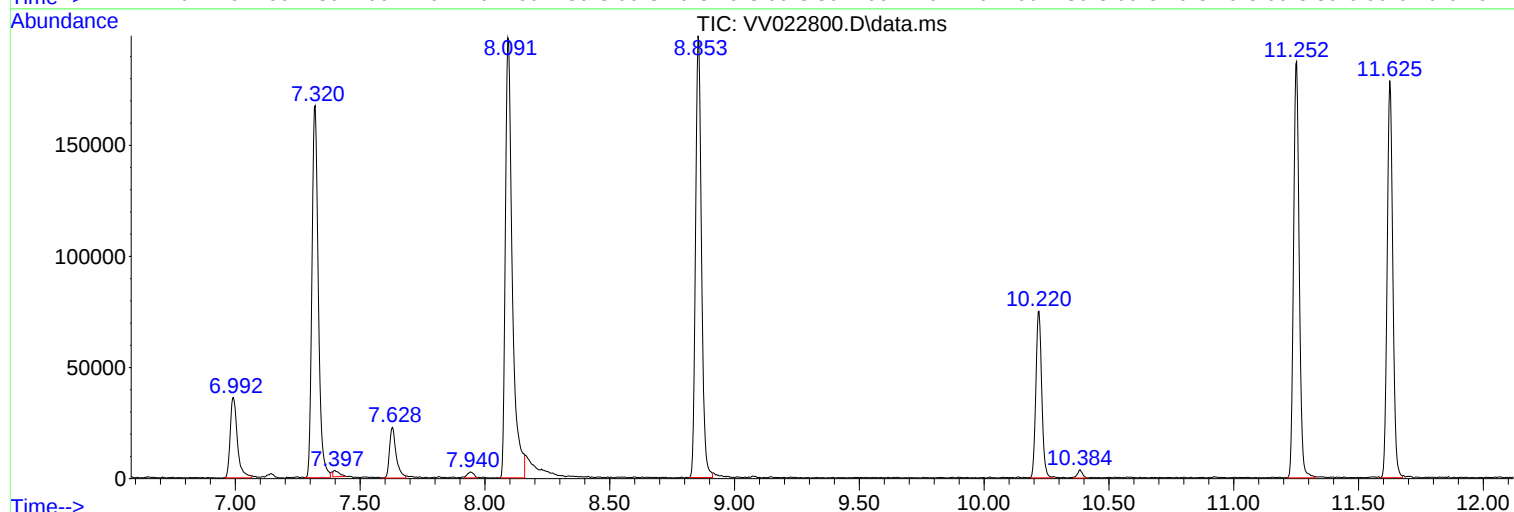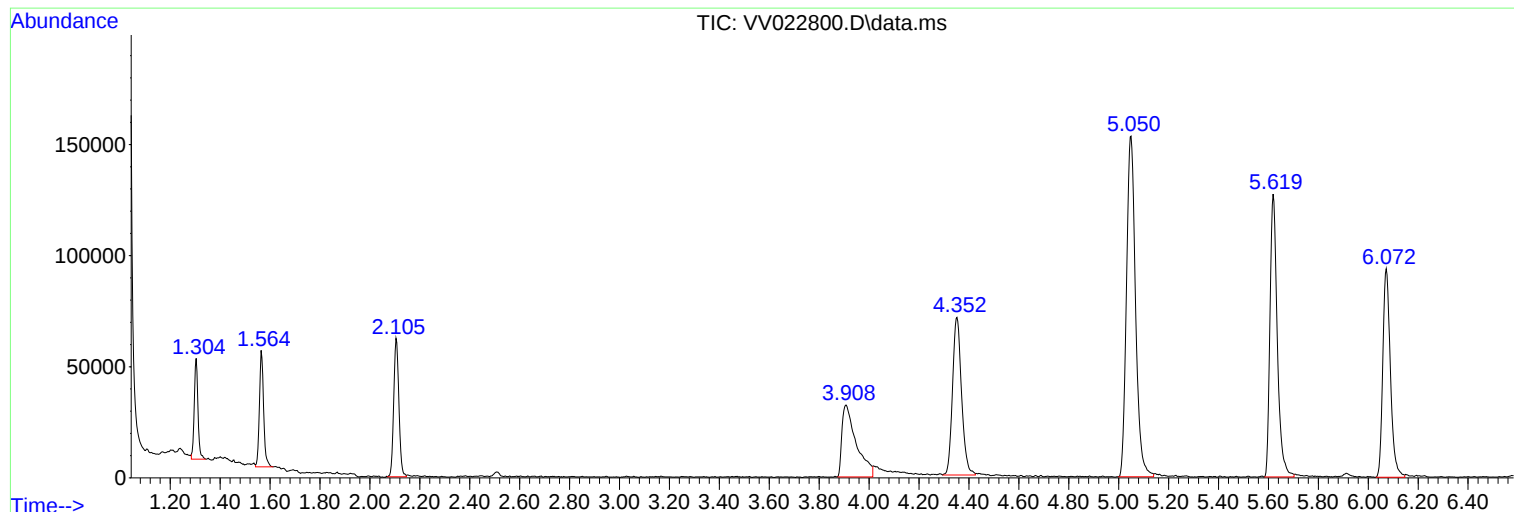

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022800.D
Acq On : 14 Oct 2021 18:16
Operator : SY/MD
Sample : M4214-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022800.D
Acq On : 14 Oct 2021 18:16
Operator : SY/MD
Sample : M4214-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
