

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022811.D
 Acq On : 14 Oct 2021 23:04
 Operator : SY/MD
 Sample : M4223-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022811.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	91	rBV	60701	63725	1.52%	0.816%
2	1.568	156	164	176	rVB	56489	64483	1.54%	0.825%
3	2.108	323	332	346	rBV	88837	128823	3.08%	1.649%
4	2.381	379	417	507	rBV	481674	4184055	100.00%	53.555%
5	3.892	874	887	923	rBV	54263	183608	4.39%	2.350%
6	4.352	1014	1030	1049	rBV	80953	201805	4.82%	2.583%
7	5.050	1231	1247	1276	rBV2	179558	453261	10.83%	5.802%
8	5.619	1410	1424	1445	rBV	130381	267667	6.40%	3.426%
9	6.072	1552	1565	1591	rBV	107673	220558	5.27%	2.823%
10	6.992	1836	1851	1870	rBV	42558	80807	1.93%	1.034%
11	7.320	1941	1953	1968	rBV	204131	366863	8.77%	4.696%
12	7.628	2039	2049	2074	rBV	25041	47574	1.14%	0.609%
13	8.091	2182	2193	2227	rBV	237587	432725	10.34%	5.539%
14	8.853	2415	2430	2455	rBV	210170	342498	8.19%	4.384%
15	10.217	2841	2854	2868	rBV	78002	125909	3.01%	1.612%
16	11.249	3165	3175	3197	rBV	208043	320503	7.66%	4.102%
17	11.625	3281	3292	3308	rBV	208296	327784	7.83%	4.196%




Sum of corrected areas: 7812648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022811.D
Acq On : 14 Oct 2021 23:04
Operator : SY/MD
Sample : M4223-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

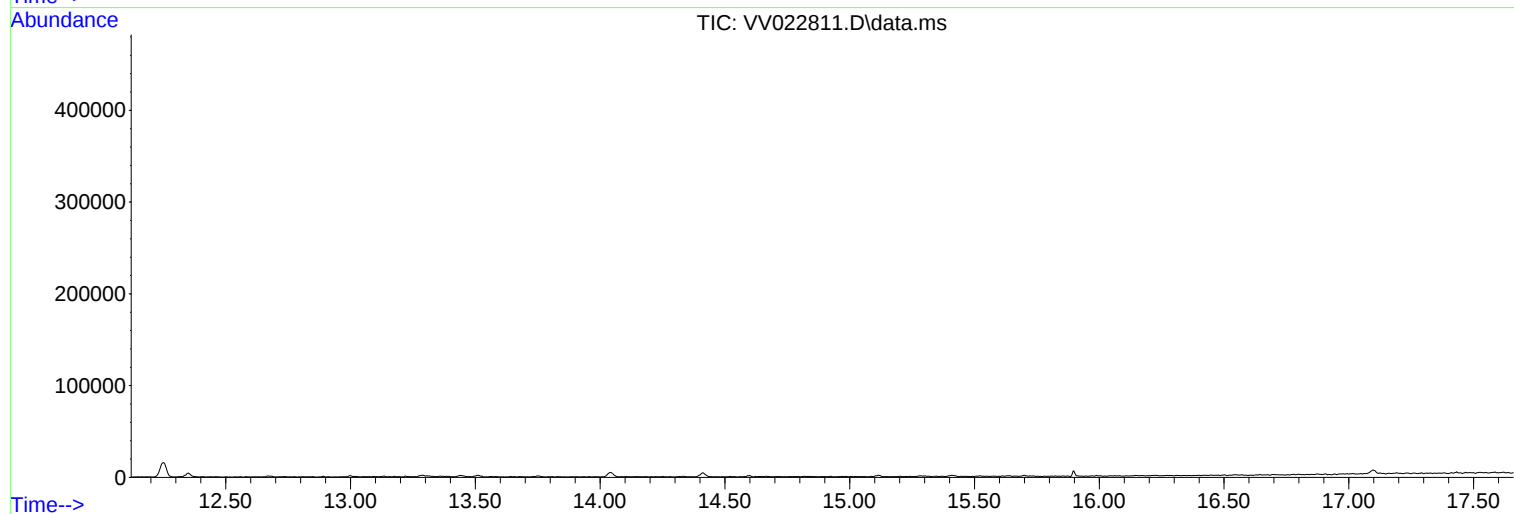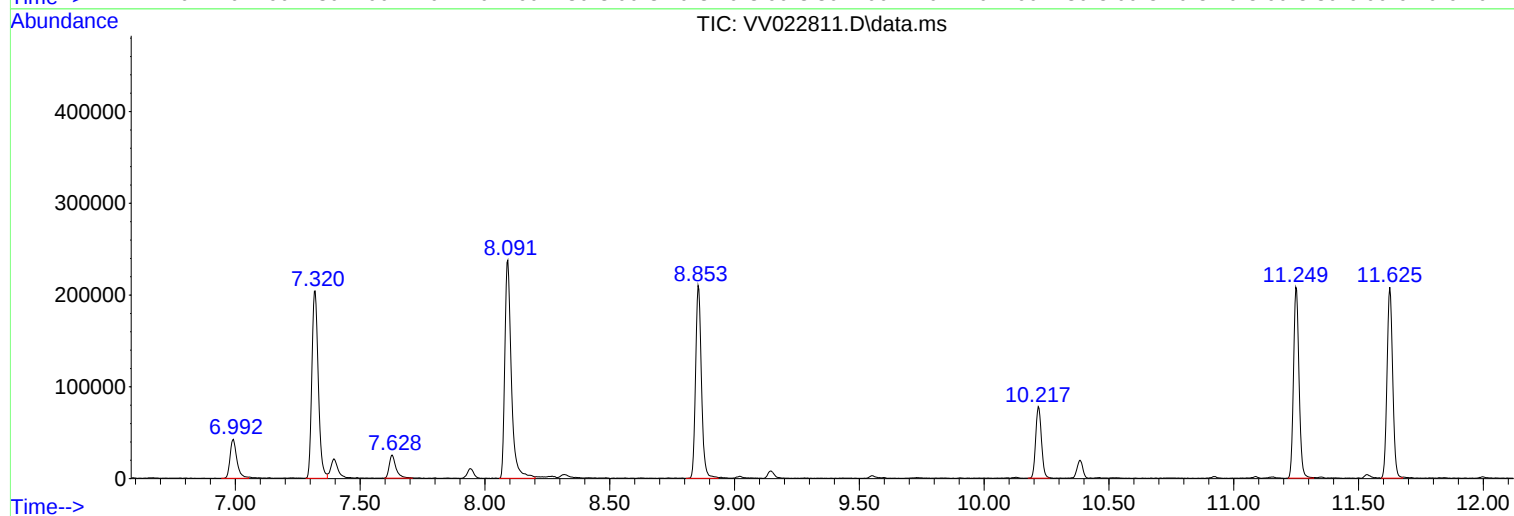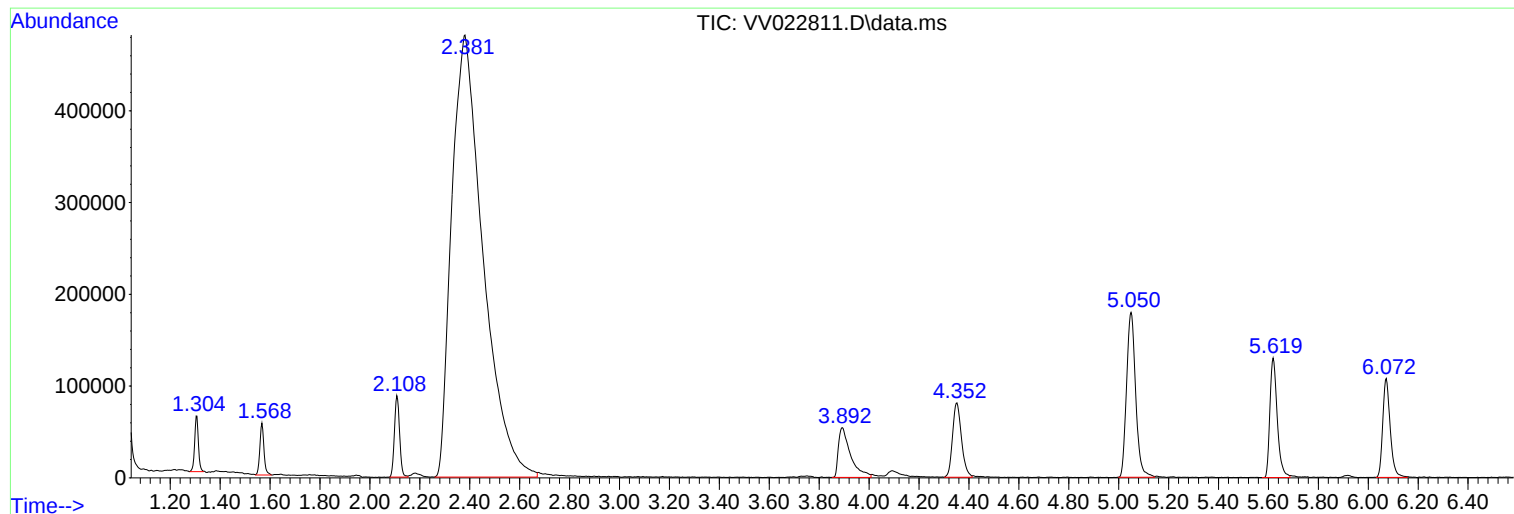

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022811.D
Acq On : 14 Oct 2021 23:04
Operator : SY/MD
Sample : M4223-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG9










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.381	78.16 ug/L	4184060	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	64

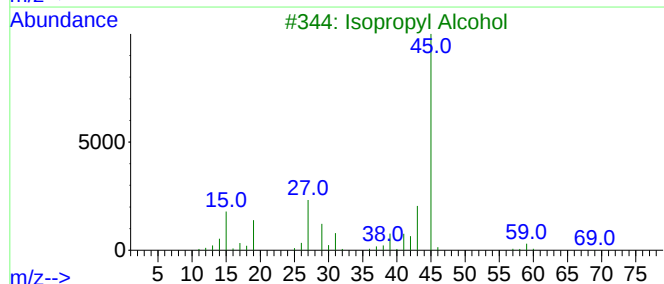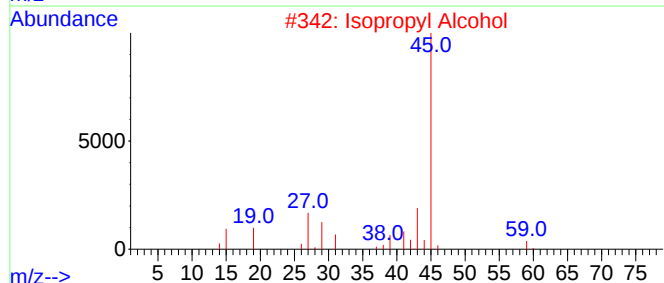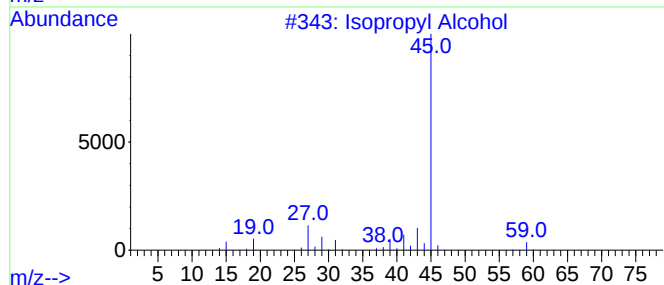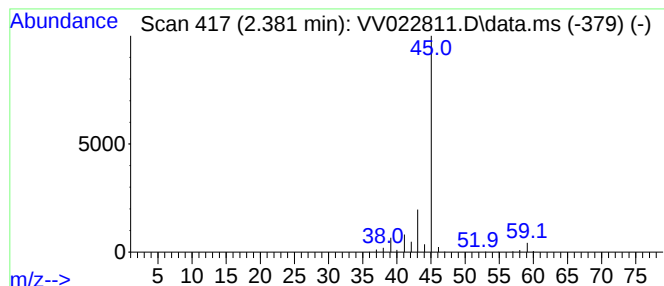

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022811.D
Acq On : 14 Oct 2021 23:04
Operator : SY/MD
Sample : M4223-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.381	78.2	ug/L	4184060	1	5.619	267667	5.0