

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022813.D
 Acq On : 14 Oct 2021 23:52
 Operator : SY/MD
 Sample : M4223-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG93

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	58920	62113	13.62%	1.693%
2	1.568	156	164	182	rVB	56334	65062	14.26%	1.773%
3	2.108	322	332	347	rBV	86521	124433	27.28%	3.392%
4	3.899	876	889	926	rBV2	54820	206465	45.26%	5.628%
5	4.352	1010	1030	1056	rBV	81722	212077	46.49%	5.781%
6	5.050	1229	1247	1273	rBV2	182251	456130	100.00%	12.433%
7	5.619	1412	1424	1451	rBV	128157	264039	57.89%	7.197%
8	5.921	1507	1518	1528	rBV9	3485	7178	1.57%	0.196%
9	6.072	1550	1565	1586	rBV	107785	217822	47.75%	5.937%
10	6.989	1840	1850	1874	rBV	43098	80201	17.58%	2.186%
11	7.320	1938	1953	1970	rBV	208631	366670	80.39%	9.994%
12	7.394	1971	1976	1990	rVB2	7152	13783	3.02%	0.376%
13	7.629	2039	2049	2065	rBV2	25258	45658	10.01%	1.244%
14	7.979	2150	2158	2172	rVB4	14619	26499	5.81%	0.722%
15	8.091	2183	2193	2221	rBV	230665	414642	90.90%	11.302%
16	8.854	2417	2430	2459	rBV	201175	334211	73.27%	9.110%
17	10.217	2842	2854	2871	rBV2	79466	126416	27.71%	3.446%
18	10.384	2897	2906	2918	rVB3	6482	11251	2.47%	0.307%
19	11.249	3160	3175	3197	rBV	196670	301633	66.13%	8.222%
20	11.625	3281	3292	3305	rBV	207311	320885	70.35%	8.746%
21	12.249	3478	3486	3497	rVB6	3570	5863	1.29%	0.160%
22	17.098	4988	4994	5000	rVB4	4199	5753	1.26%	0.157%


Sum of corrected areas: 3668784

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022813.D
Acq On : 14 Oct 2021 23:52
Operator : SY/MD
Sample : M4223-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

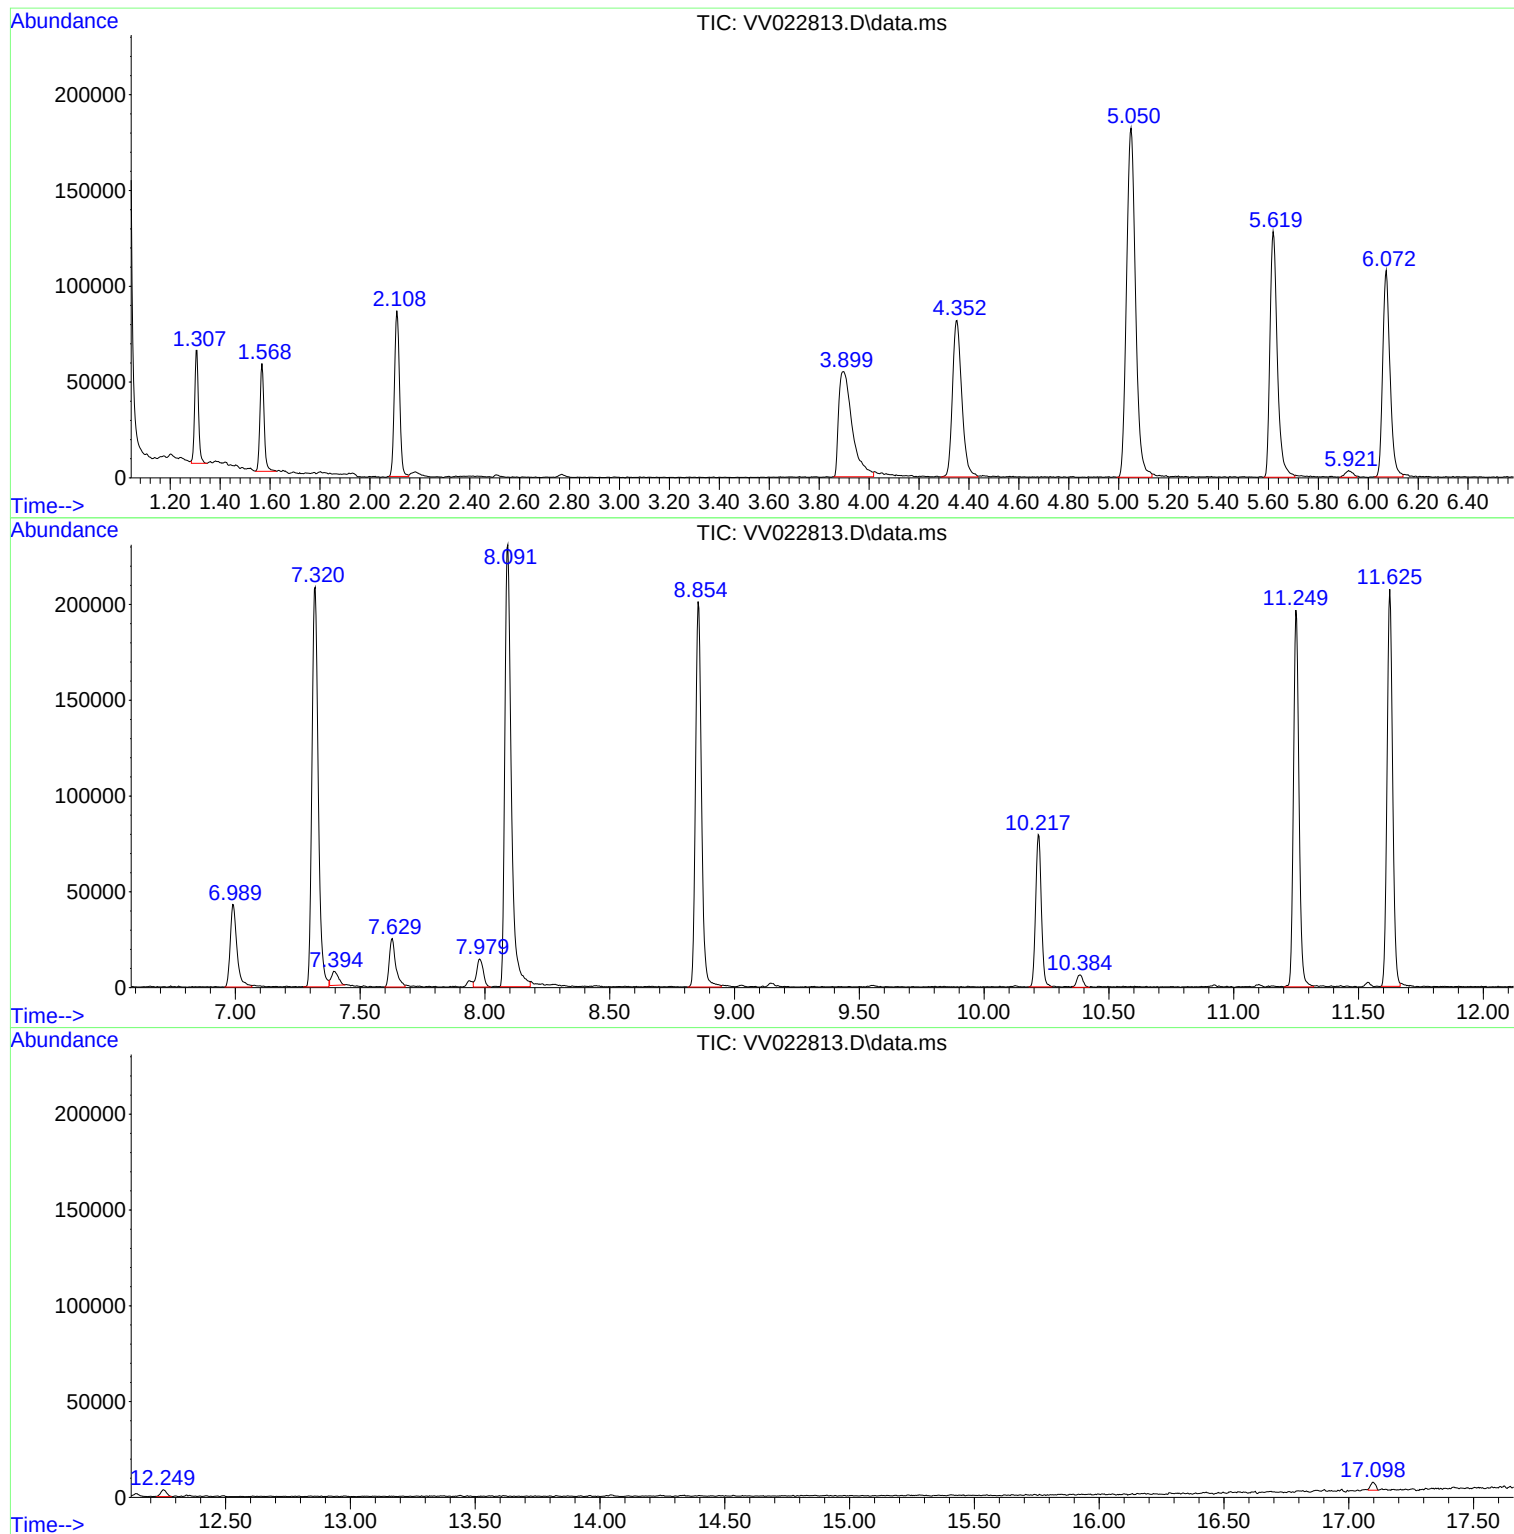

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022813.D
Acq On : 14 Oct 2021 23:52
Operator : SY/MD
Sample : M4223-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022813.D
Acq On : 14 Oct 2021 23:52
Operator : SY/MD
Sample : M4223-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
