

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022814.D
 Acq On : 15 Oct 2021 00:16
 Operator : SY/MD
 Sample : M4223-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG94

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	61926	65193	13.94%	1.773%
2	1.568	156	164	173	rVB	57709	64013	13.69%	1.741%
3	2.108	321	332	349	rBV	90857	130984	28.01%	3.562%
4	3.892	876	887	930	rBV2	50748	173705	37.14%	4.724%
5	4.349	1012	1029	1051	rBV	83665	209512	44.80%	5.698%
6	5.050	1231	1247	1278	rBV2	186847	467668	100.00%	12.718%
7	5.619	1410	1424	1445	rBV	127097	259661	55.52%	7.062%
8	6.072	1552	1565	1588	rBV	108646	225887	48.30%	6.143%
9	6.989	1839	1850	1873	rBV	44074	84154	17.99%	2.289%
10	7.317	1939	1952	1969	rBV	211447	372527	79.66%	10.131%
11	7.397	1970	1977	1993	rVB2	10197	20586	4.40%	0.560%
12	7.628	2039	2049	2066	rBV	25397	46931	10.04%	1.276%
13	7.940	2135	2146	2154	rBV5	3063	5811	1.24%	0.158%
14	8.091	2183	2193	2221	rBV	235438	421570	90.14%	11.465%
15	8.853	2419	2430	2451	rBV	203684	332802	71.16%	9.051%
16	9.146	2511	2521	2532	rBV6	5202	8620	1.84%	0.234%
17	10.217	2842	2854	2872	rBV	84109	130437	27.89%	3.547%
18	10.384	2897	2906	2923	rVB2	6289	10551	2.26%	0.287%
19	11.249	3164	3175	3191	rBV	196467	305794	65.39%	8.316%
20	11.625	3281	3292	3312	rBV	216701	335779	71.80%	9.132%
21	12.249	3479	3486	3496	rBV3	3164	4924	1.05%	0.134%


Sum of corrected areas: 3677109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022814.D
Acq On : 15 Oct 2021 00:16
Operator : SY/MD
Sample : M4223-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

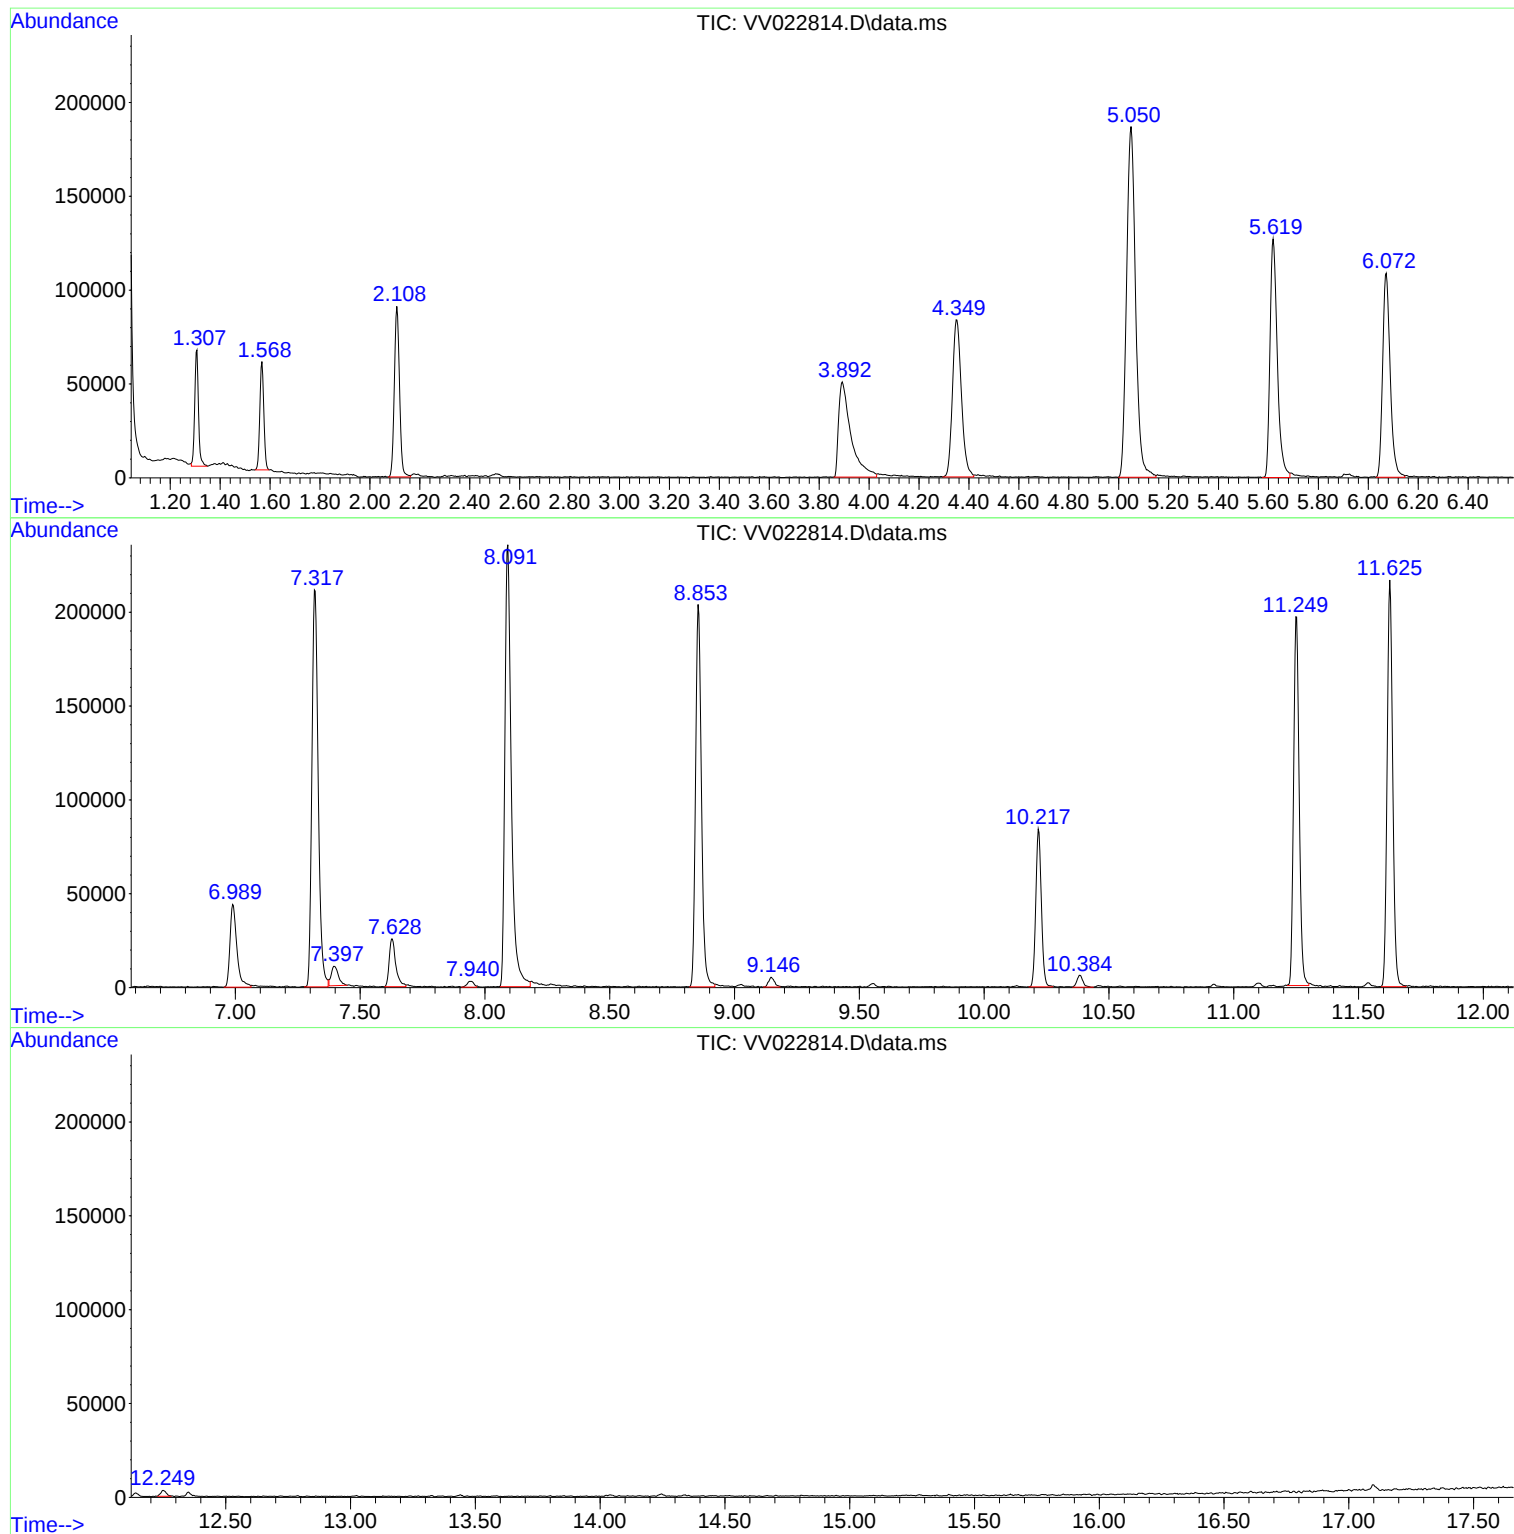

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022814.D
Acq On : 15 Oct 2021 00:16
Operator : SY/MD
Sample : M4223-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022814.D
Acq On : 15 Oct 2021 00:16
Operator : SY/MD
Sample : M4223-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------