

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022818.D
 Acq On : 15 Oct 2021 01:51
 Operator : SY/MD
 Sample : M4223-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG98

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	200232	210348	11.89%	1.633%
2	1.568	156	164	175	rBV	178973	193171	10.92%	1.499%
3	2.108	321	332	347	rBV	261097	376619	21.30%	2.923%
4	2.770	524	538	554	rBV	15754	32925	1.86%	0.256%
5	3.912	879	893	919	rBV4	55746	183402	10.37%	1.424%
6	4.349	1009	1029	1058	rBV	244224	607158	34.33%	4.713%
7	5.047	1229	1246	1274	rBV2	517415	1301592	73.60%	10.103%
8	5.616	1410	1423	1455	rBV	624561	1243020	70.29%	9.649%
9	5.918	1506	1517	1537	rVB4	23935	52817	2.99%	0.410%
10	6.069	1548	1564	1592	rBV	386178	775938	43.88%	6.023%
11	6.985	1837	1849	1874	rBV	187636	339430	19.19%	2.635%
12	7.317	1940	1952	1968	rBV	757706	1288725	72.87%	10.004%
13	7.394	1969	1976	1990	rVB2	18436	36787	2.08%	0.286%
14	7.622	2037	2047	2068	rBV	117696	203544	11.51%	1.580%
15	7.976	2136	2157	2179	rBV	188989	333495	18.86%	2.589%
16	8.092	2183	2193	2215	rBV	172868	312633	17.68%	2.427%
17	8.854	2417	2430	2450	rBV	1086769	1739993	98.39%	13.507%
18	10.217	2839	2854	2870	rBV	333869	509519	28.81%	3.955%
19	10.384	2894	2906	2918	rVB2	12484	19475	1.10%	0.151%
20	11.249	3163	3175	3199	rBV	1180786	1768469	100.00%	13.728%
21	11.625	3279	3292	3315	rBV	875217	1353540	76.54%	10.507%




Sum of corrected areas: 12882600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022818.D
Acq On : 15 Oct 2021 01:51
Operator : SY/MD
Sample : M4223-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

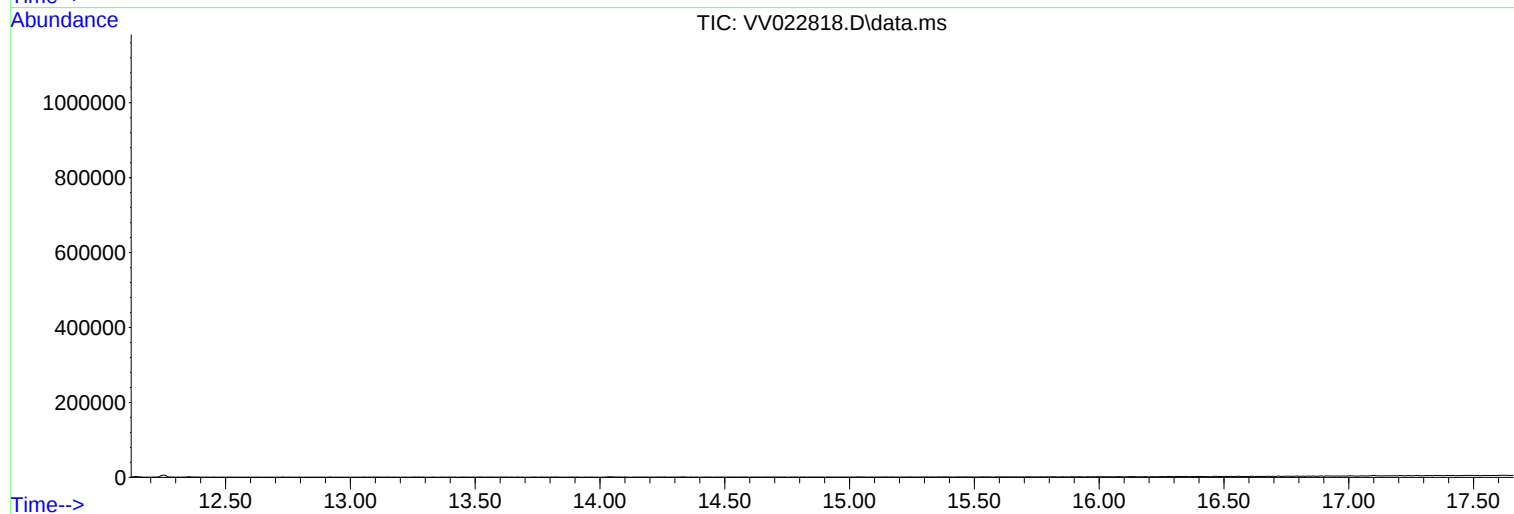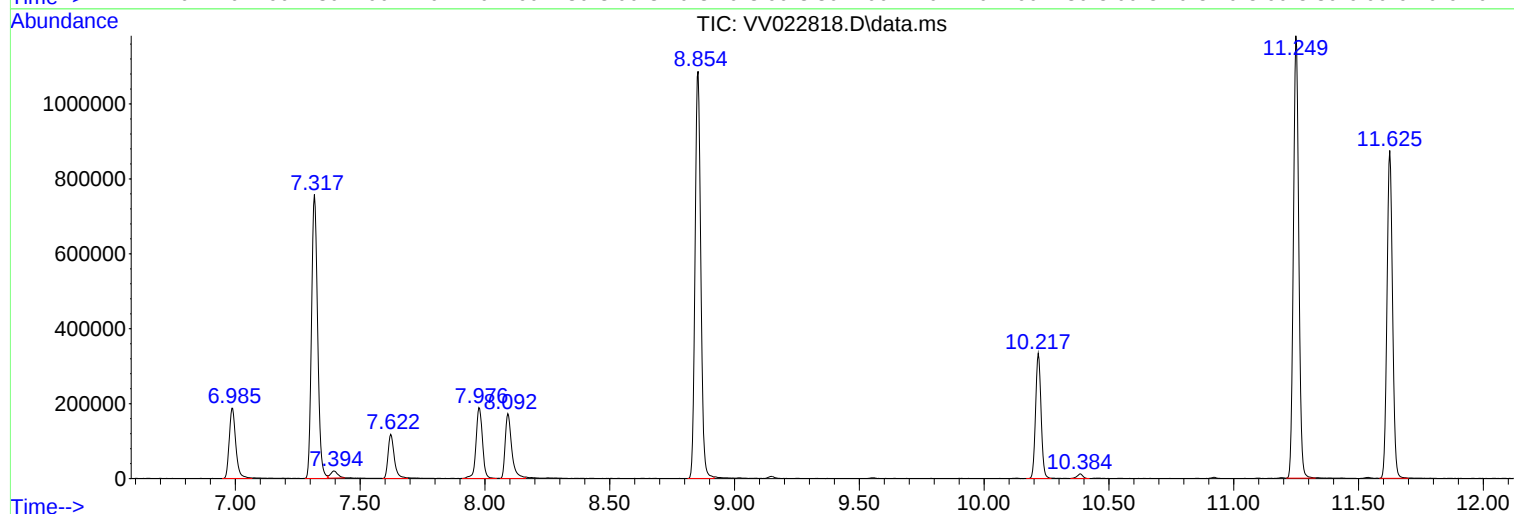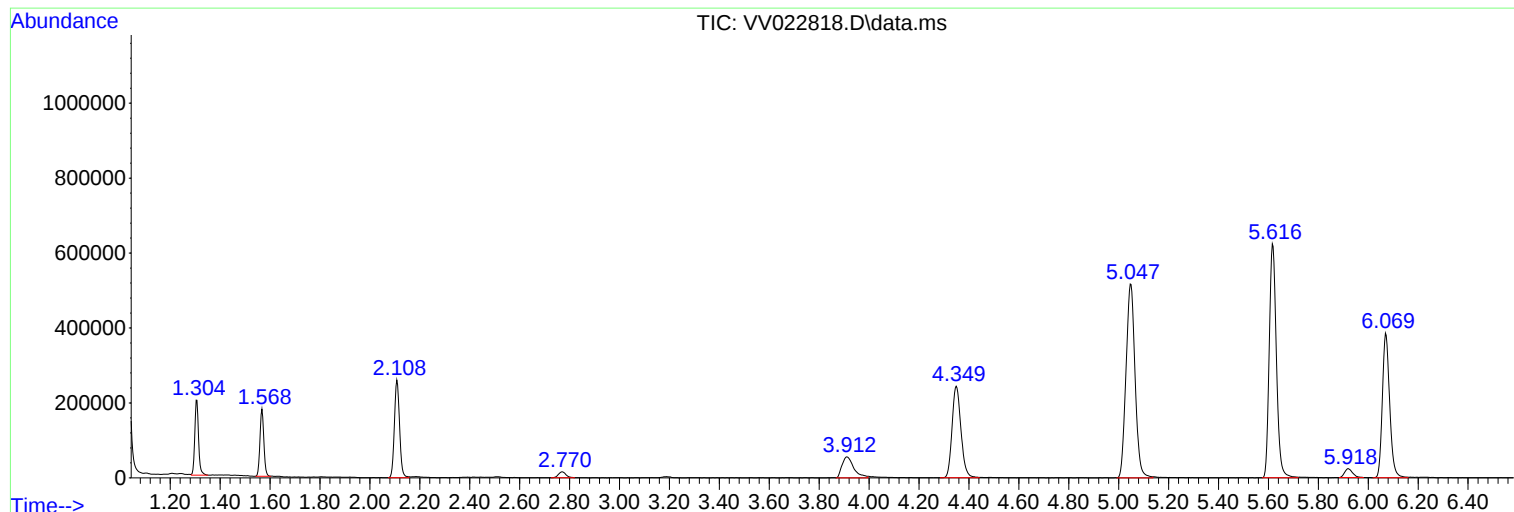

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022818.D
Acq On : 15 Oct 2021 01:51
Operator : SY/MD
Sample : M4223-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022818.D
Acq On : 15 Oct 2021 01:51
Operator : SY/MD
Sample : M4223-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
