

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022819.D
 Acq On : 15 Oct 2021 02:15
 Operator : SY/MD
 Sample : M4223-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG99

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rVB	216447	220191	12.43%	1.620%
2	1.568	156	164	176	rVB	187983	205299	11.59%	1.510%
3	2.108	316	332	351	rBV	348142	496889	28.06%	3.655%
4	3.902	878	890	924	rBV2	38997	145733	8.23%	1.072%
5	4.349	1012	1029	1058	rBV	305743	756488	42.71%	5.564%
6	5.047	1223	1246	1275	rBV2	645770	1632091	92.15%	12.004%
7	5.616	1408	1423	1459	rBV	738778	1453683	82.08%	10.692%
8	5.918	1502	1517	1533	rBV7	7458	18148	1.02%	0.133%
9	6.069	1549	1564	1591	rBV	404203	820437	46.32%	6.034%
10	6.985	1838	1849	1872	rBV	194233	354636	20.02%	2.608%
11	7.317	1939	1952	1969	rBV	803056	1365418	77.09%	10.043%
12	7.394	1970	1976	1995	rVB	17452	36691	2.07%	0.270%
13	7.622	2037	2047	2069	rBV	124037	214394	12.11%	1.577%
14	7.979	2149	2158	2172	rVB2	30168	52480	2.96%	0.386%
15	8.091	2182	2193	2219	rBV	180019	328382	18.54%	2.415%
16	8.853	2418	2430	2457	rBV	1097447	1759002	99.32%	12.938%
17	10.217	2841	2854	2873	rBV	344432	533434	30.12%	3.923%
18	11.249	3163	3175	3203	rBV	1188117	1771116	100.00%	13.027%
19	11.625	3277	3292	3313	rBV	931843	1431419	80.82%	10.528%




Sum of corrected areas: 13595931

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022819.D
Acq On : 15 Oct 2021 02:15
Operator : SY/MD
Sample : M4223-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

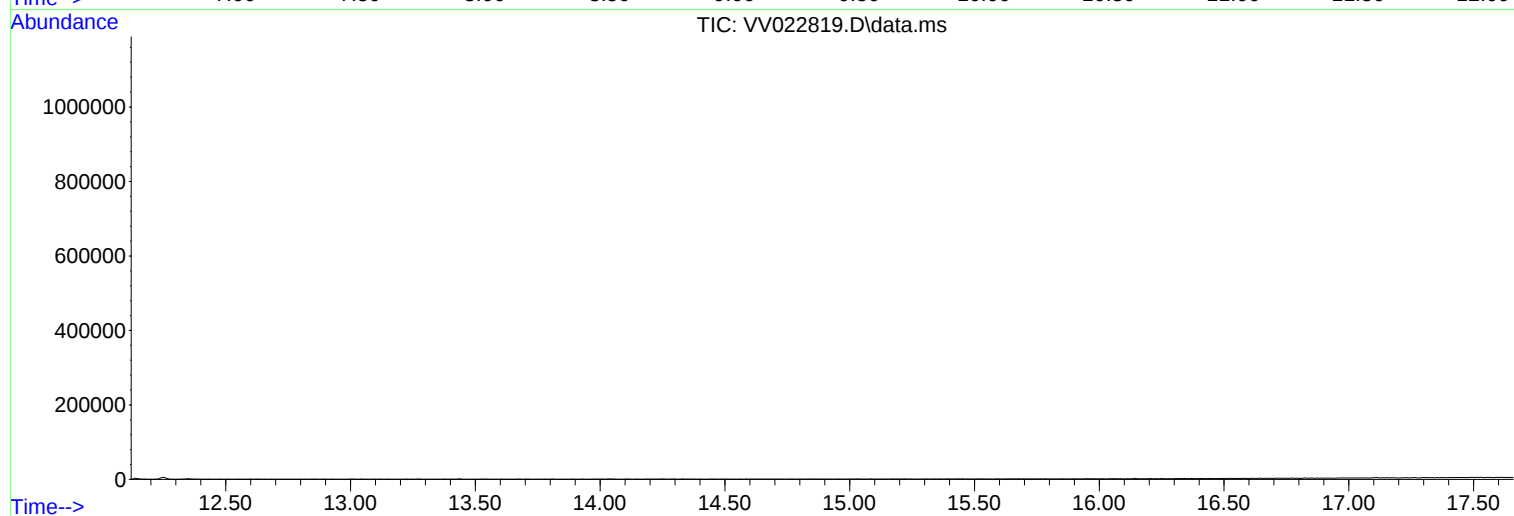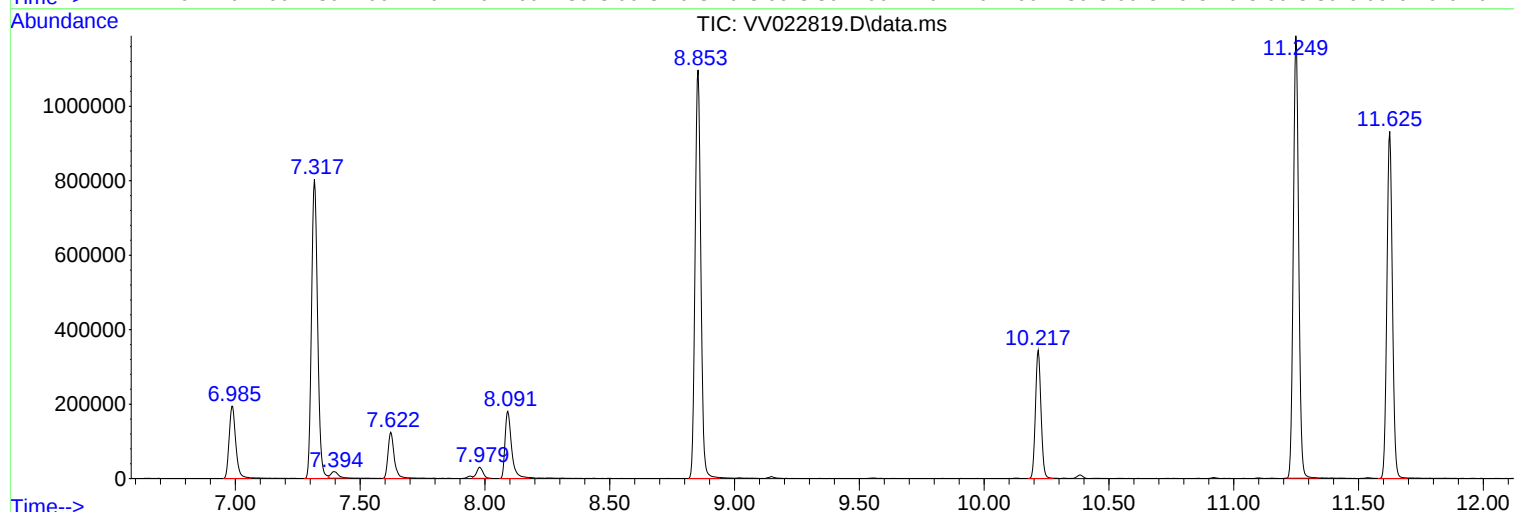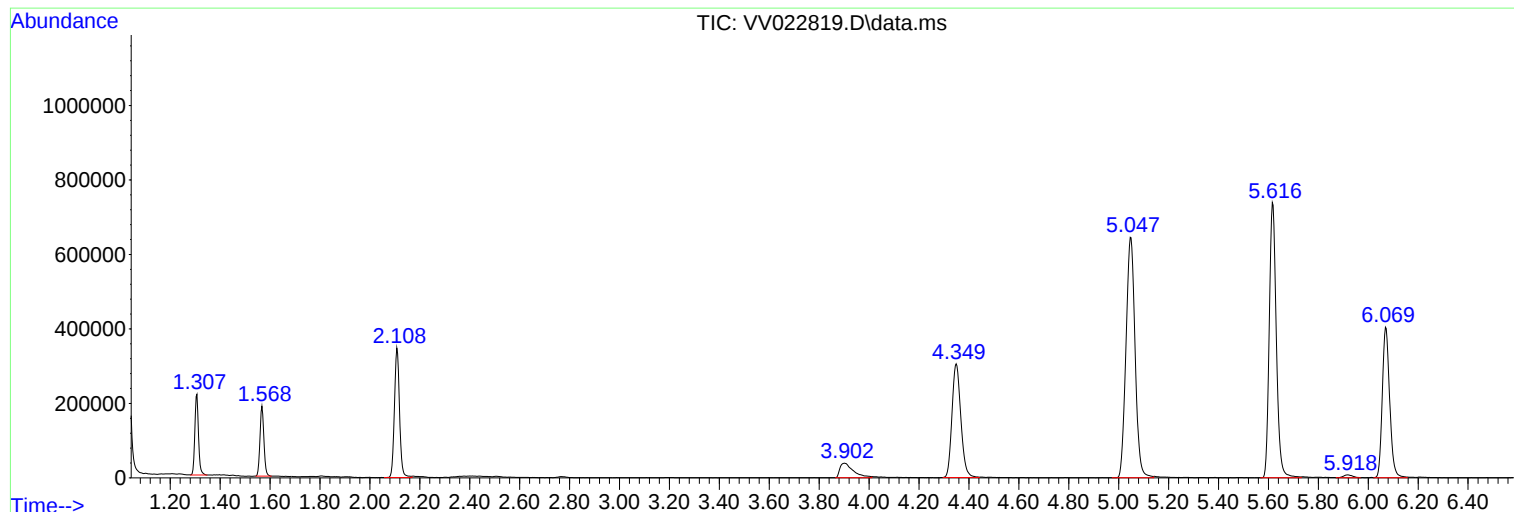

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022819.D
Acq On : 15 Oct 2021 02:15
Operator : SY/MD
Sample : M4223-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022819.D
Acq On : 15 Oct 2021 02:15
Operator : SY/MD
Sample : M4223-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
