

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022820.D
 Acq On : 15 Oct 2021 02:39
 Operator : SY/MD
 Sample : M4223-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGA0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	197899	206990	11.71%	1.583%
2	1.568	156	164	179	rBV	150945	171028	9.67%	1.308%
3	2.108	321	332	353	rBV	285310	412332	23.32%	3.154%
4	3.905	878	891	917	rBV2	32886	120650	6.82%	0.923%
5	4.349	1010	1029	1065	rBV	299851	797010	45.07%	6.097%
6	5.047	1228	1246	1276	rBV2	619077	1557032	88.05%	11.911%
7	5.616	1410	1423	1461	rBV	730807	1447371	81.85%	11.072%
8	6.069	1551	1564	1590	rBV	382888	776812	43.93%	5.943%
9	6.985	1838	1849	1876	rBV	189967	343375	19.42%	2.627%
10	7.317	1939	1952	1969	rBV	761641	1292839	73.11%	9.890%
11	7.397	1970	1977	1990	rVB2	14581	28039	1.59%	0.214%
12	7.622	2037	2047	2071	rBV	118080	206219	11.66%	1.578%
13	7.979	2151	2158	2171	rVB3	18119	32426	1.83%	0.248%
14	8.091	2182	2193	2219	rBV	170526	313550	17.73%	2.399%
15	8.853	2417	2430	2451	rBV	1082645	1736963	98.22%	13.288%
16	10.217	2839	2854	2880	rBV	323034	508371	28.75%	3.889%
17	11.249	3162	3175	3198	rBV	1175082	1768380	100.00%	13.528%
18	11.625	3278	3292	3314	rBV	872507	1352411	76.48%	10.346%




Sum of corrected areas: 13071798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022820.D
Acq On : 15 Oct 2021 02:39
Operator : SY/MD
Sample : M4223-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

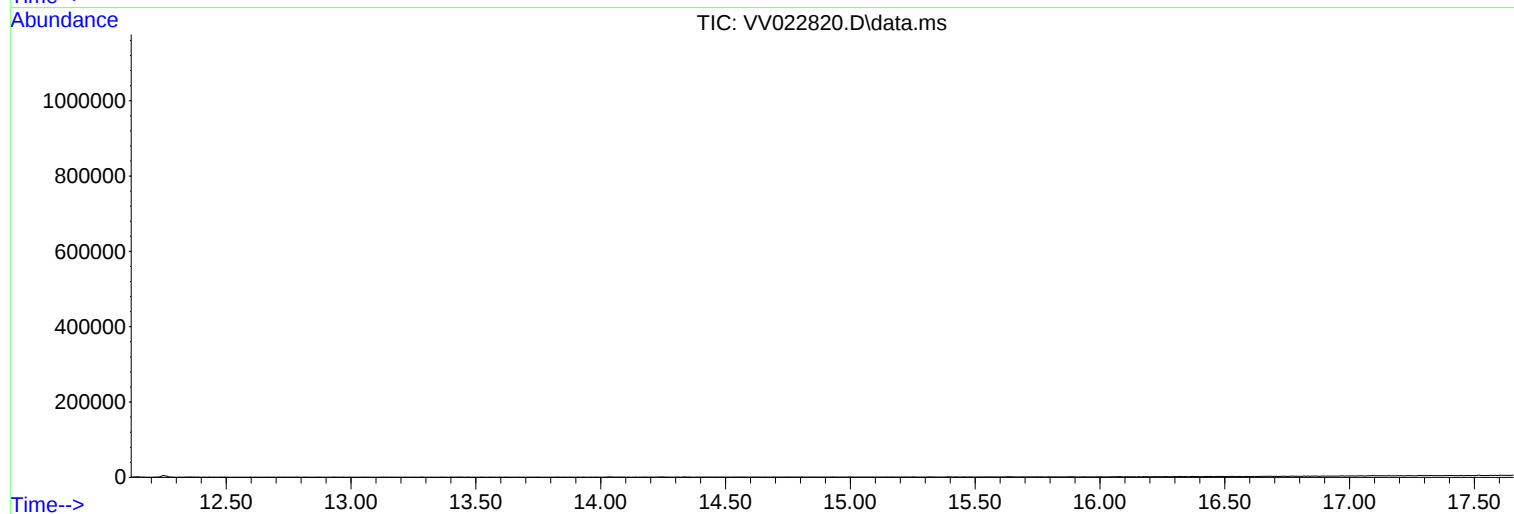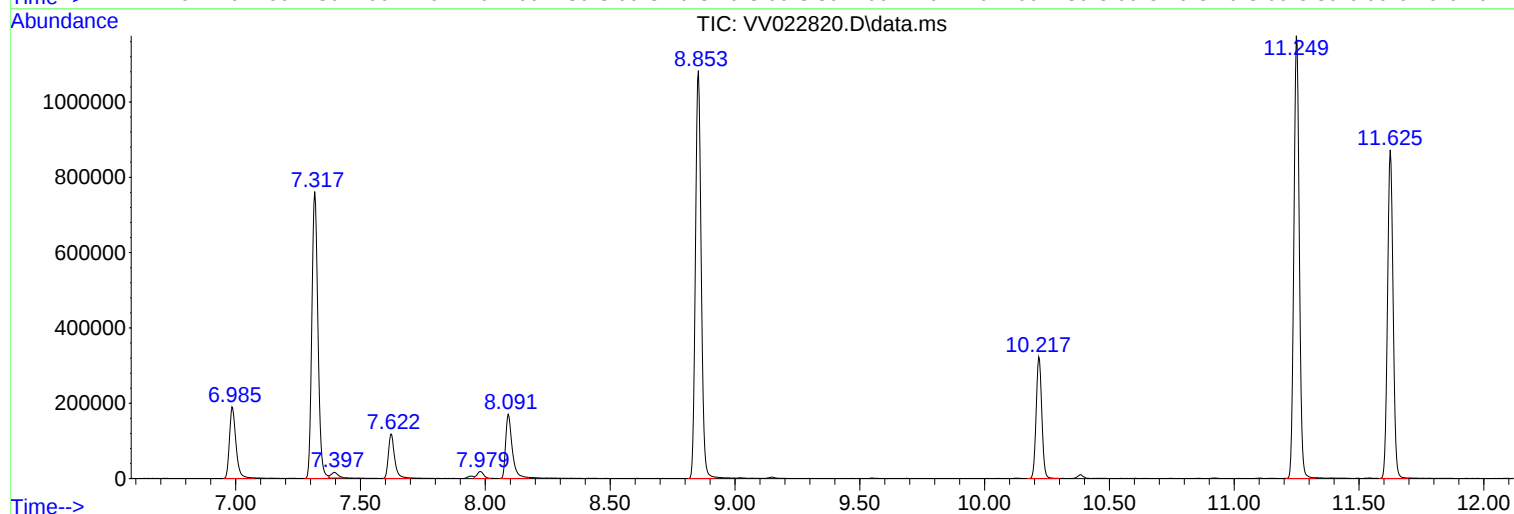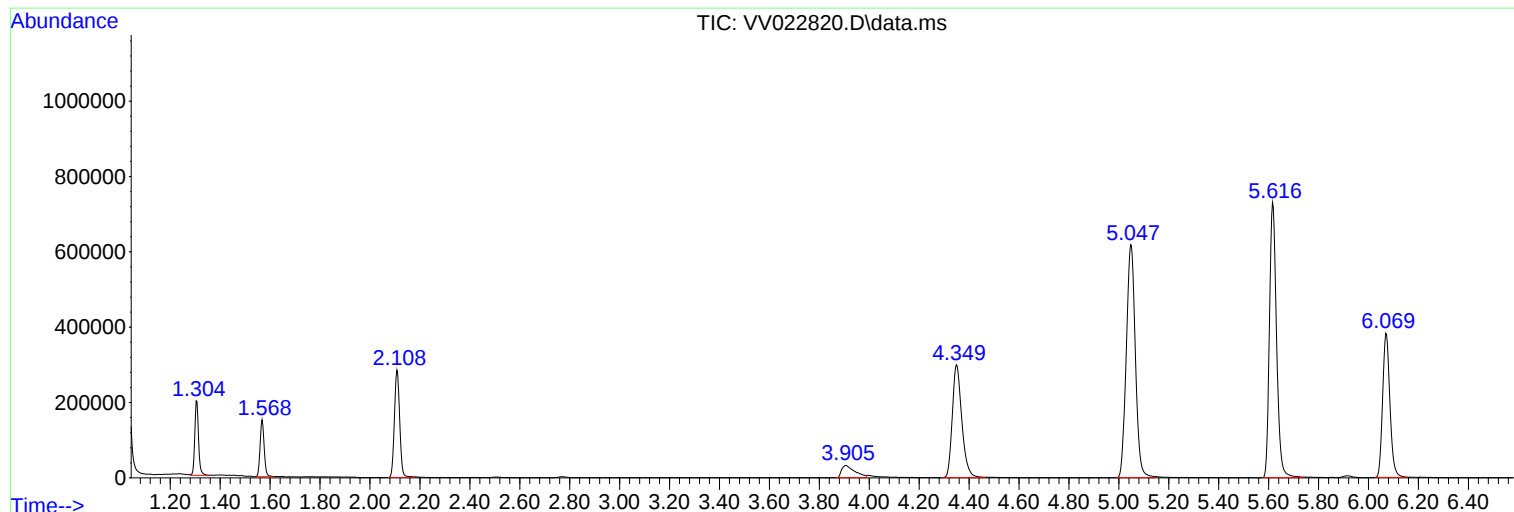

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022820.D
Acq On : 15 Oct 2021 02:39
Operator : SY/MD
Sample : M4223-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022820.D
Acq On : 15 Oct 2021 02:39
Operator : SY/MD
Sample : M4223-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
