

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022823.D
 Acq On : 15 Oct 2021 03:51
 Operator : SY/MD
 Sample : M4223-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGC4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB2	74916	78926	3.59%	1.113%
2	1.568	156	164	179	rVB	58895	66713	3.04%	0.941%
3	2.108	320	332	347	rBV	86439	125199	5.70%	1.766%
4	2.368	382	413	414	rBV4	24423	74855	3.41%	1.056%
5	2.767	522	537	551	rBV2	18217	37656	1.71%	0.531%
6	3.912	876	893	927	rBV2	345548	911981	41.50%	12.863%
7	4.352	1014	1030	1058	rBV2	69987	181041	8.24%	2.554%
8	5.050	1231	1247	1274	rBV2	157956	396610	18.05%	5.594%
9	5.619	1412	1424	1449	rBV	137466	283038	12.88%	3.992%
10	5.915	1504	1516	1543	rBV	149969	302393	13.76%	4.265%
11	6.072	1552	1565	1585	rBV	111101	225020	10.24%	3.174%
12	6.992	1836	1851	1865	rBV	44032	81767	3.72%	1.153%
13	7.317	1941	1952	1970	rBV	214714	381524	17.36%	5.381%
14	7.625	2039	2048	2069	rBV2	26029	48436	2.20%	0.683%
15	7.976	2135	2157	2183	rBV	1324807	2197807	100.00%	30.999%
16	8.092	2183	2193	2217	rVV	255776	449683	20.46%	6.343%
17	8.854	2417	2430	2461	rBV	218894	365179	16.62%	5.151%
18	10.220	2844	2855	2869	rBV	82692	131521	5.98%	1.855%
19	10.384	2895	2906	2919	rVB2	16684	25947	1.18%	0.366%
20	11.249	3165	3175	3194	rVV	221677	355683	16.18%	5.017%
21	11.625	3281	3292	3312	rVV	225844	368857	16.78%	5.203%




Sum of corrected areas: 7089836

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022823.D
Acq On : 15 Oct 2021 03:51
Operator : SY/MD
Sample : M4223-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

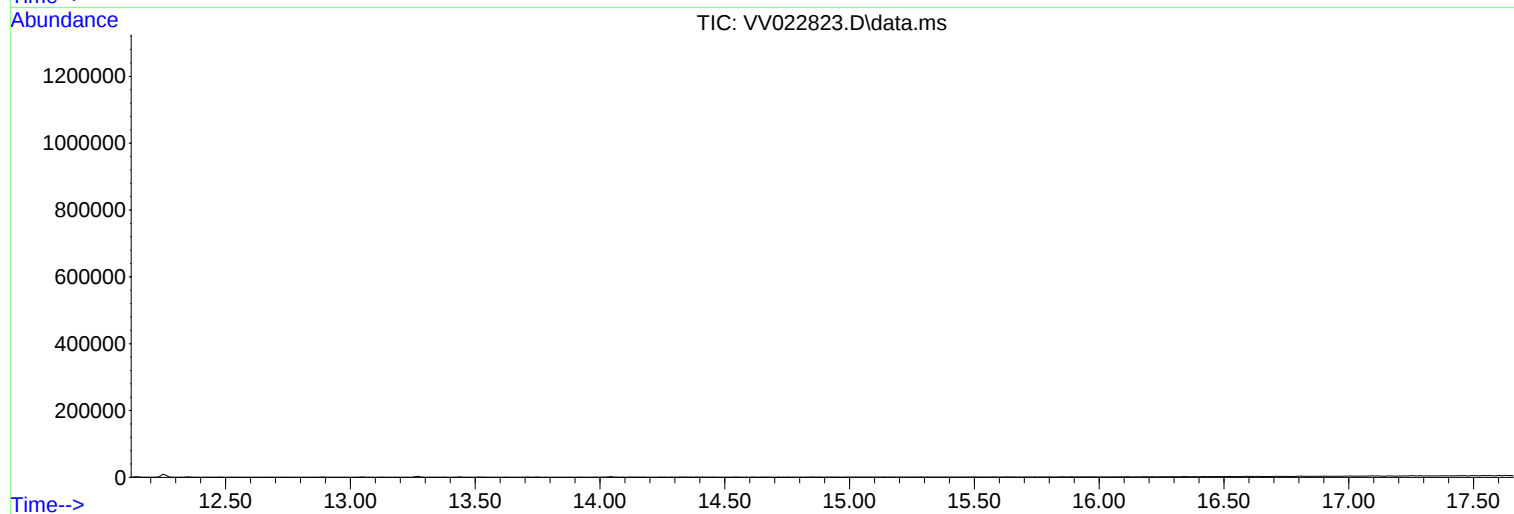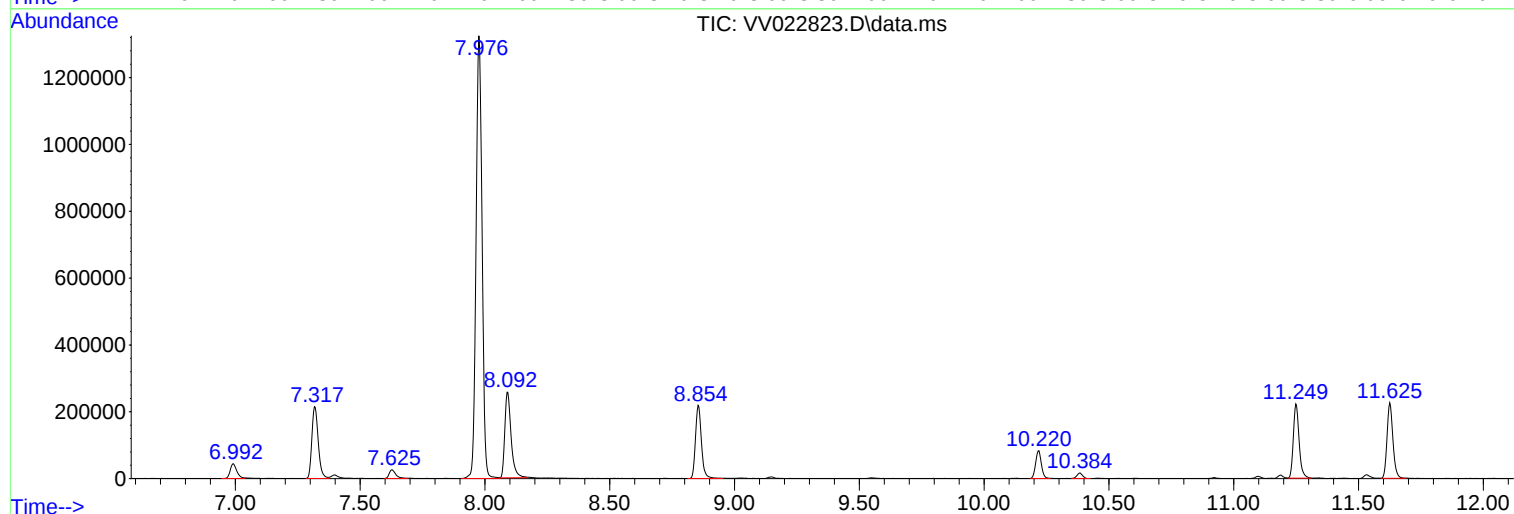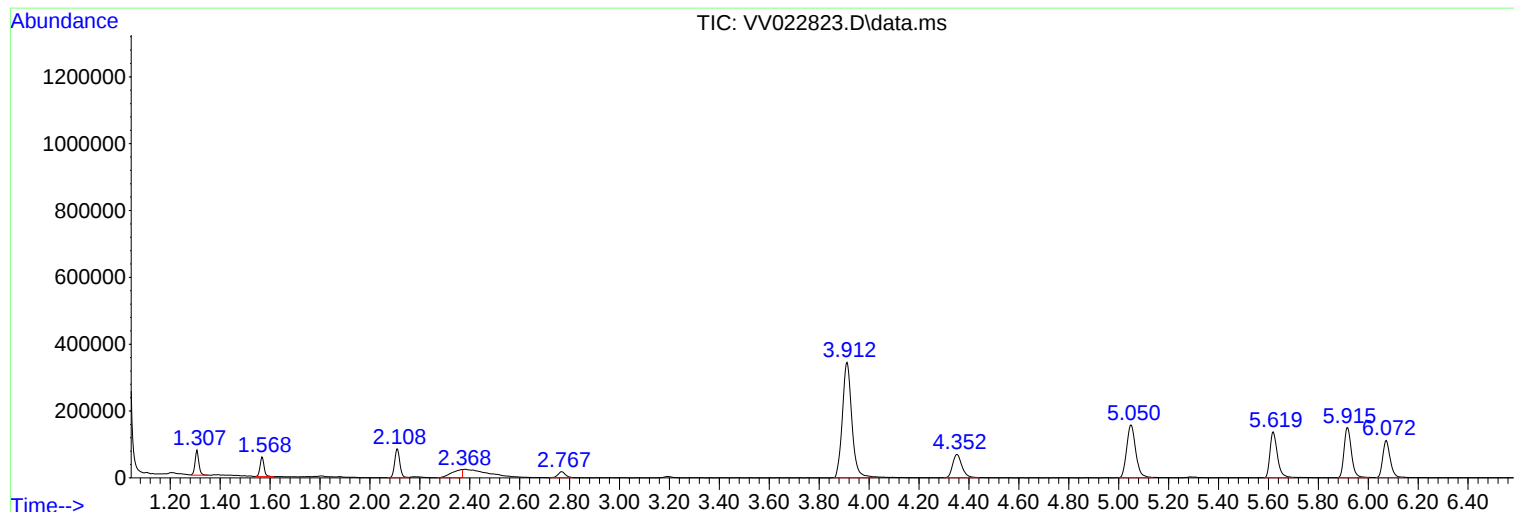

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022823.D
Acq On : 15 Oct 2021 03:51
Operator : SY/MD
Sample : M4223-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.368	1.32 ug/L	74855	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	74
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	9
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	9
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

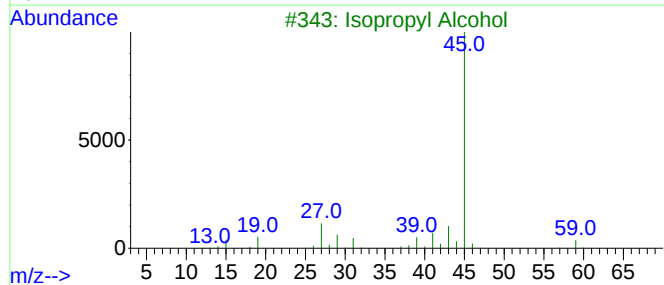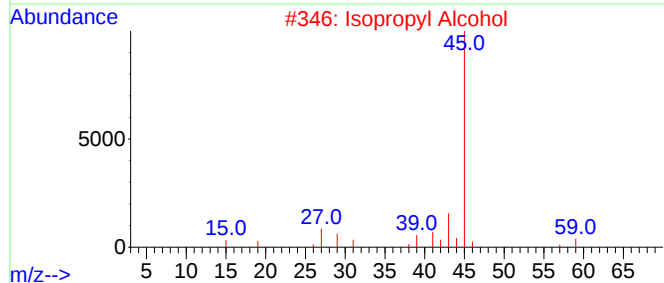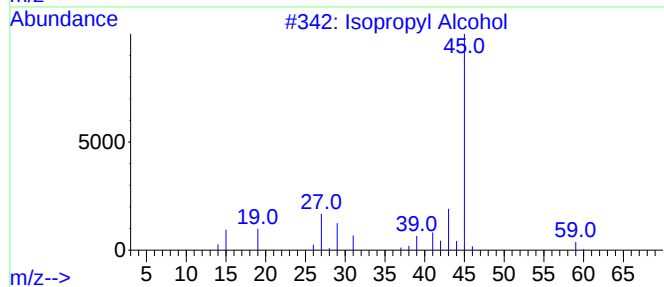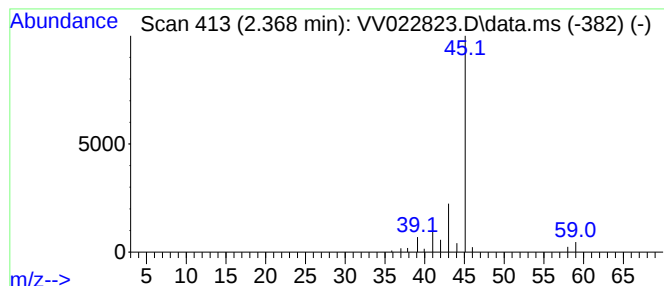

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022823.D
Acq On : 15 Oct 2021 03:51
Operator : SY/MD
Sample : M4223-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.368	1.3	ug/L	74855	1	5.619	283038	5.0