

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022825.D
 Acq On : 15 Oct 2021 04:39
 Operator : SY/MD
 Sample : M4223-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGC6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	29	rVB	8155	8287	1.39%	0.185%
2	1.307	76	83	97	rVB	60404	64847	10.87%	1.451%
3	1.568	158	164	177	rVB	48192	53946	9.05%	1.207%
4	2.108	322	332	344	rBV	102774	149479	25.07%	3.345%
5	2.179	344	354	381	rVB	18372	46398	7.78%	1.038%
6	2.767	523	537	550	rBV2	21553	43775	7.34%	0.980%
7	3.909	872	892	922	rBV3	58354	222911	37.38%	4.989%
8	4.352	1014	1030	1053	rBV	83395	208086	34.90%	4.657%
9	5.050	1230	1247	1276	rBV2	185271	464164	77.84%	10.388%
10	5.619	1413	1424	1453	rBV	133563	275170	46.14%	6.159%
11	5.921	1506	1518	1542	rVB3	24957	54719	9.18%	1.225%
12	6.072	1551	1565	1586	rBV	107642	221595	37.16%	4.960%
13	6.989	1840	1850	1871	rBV	41719	79825	13.39%	1.787%
14	7.317	1939	1952	1969	rBV	214742	376928	63.21%	8.436%
15	7.397	1971	1977	1990	rVB4	5997	12919	2.17%	0.289%
16	7.629	2039	2049	2065	rBV	24913	45122	7.57%	1.010%
17	7.976	2136	2157	2174	rBV	349309	596320	100.00%	13.346%
18	8.092	2183	2193	2214	rBV	210153	376798	63.19%	8.433%
19	8.854	2418	2430	2453	rBV	213482	350180	58.72%	7.837%
20	9.143	2509	2520	2533	rVB8	3942	7130	1.20%	0.160%
21	10.217	2842	2854	2871	rBV	75474	120306	20.17%	2.693%
22	10.384	2893	2906	2916	rVB2	9213	14404	2.42%	0.322%
23	10.921	3064	3073	3082	rBV2	4716	6403	1.07%	0.143%
24	11.252	3162	3176	3197	rBV	209537	323690	54.28%	7.245%
25	11.625	3281	3292	3314	rVB	215334	335155	56.20%	7.501%
26	12.252	3476	3487	3497	rVB2	5791	9513	1.60%	0.213%




Sum of corrected areas: 4468070

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022825.D
Acq On : 15 Oct 2021 04:39
Operator : SY/MD
Sample : M4223-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

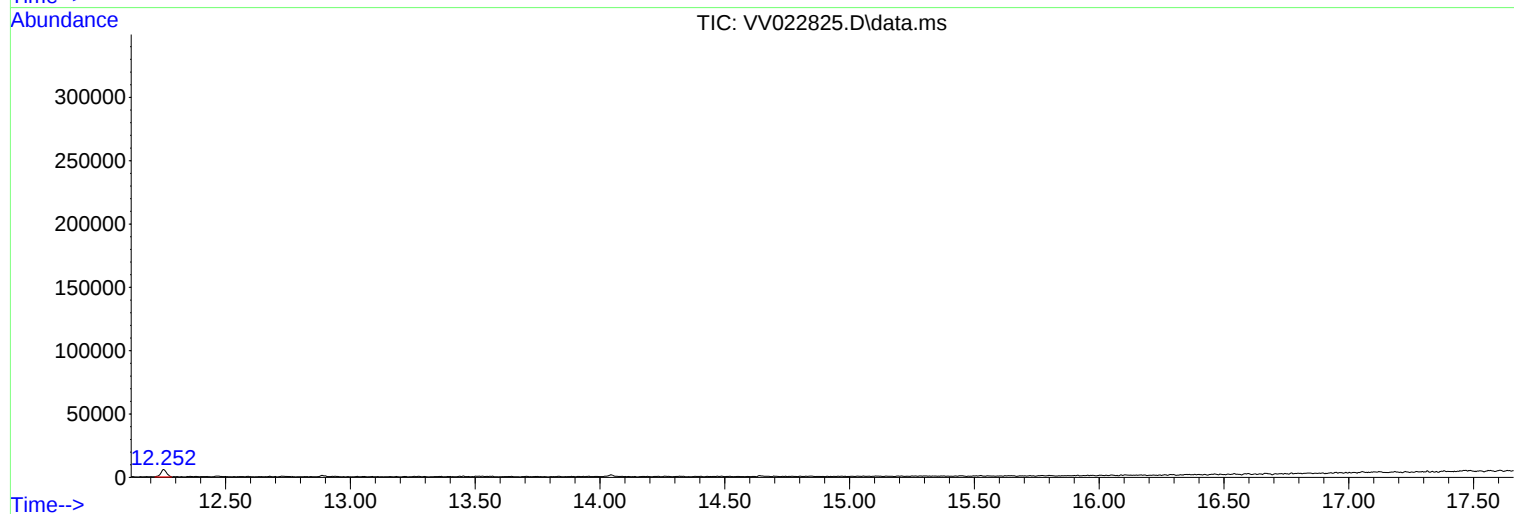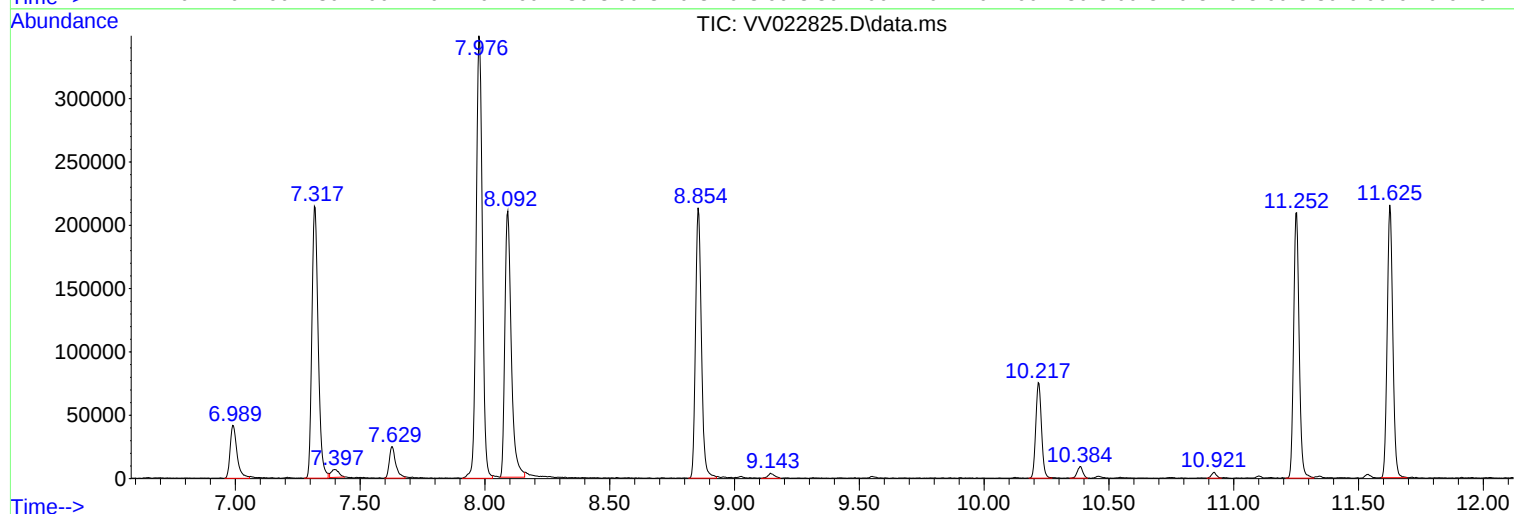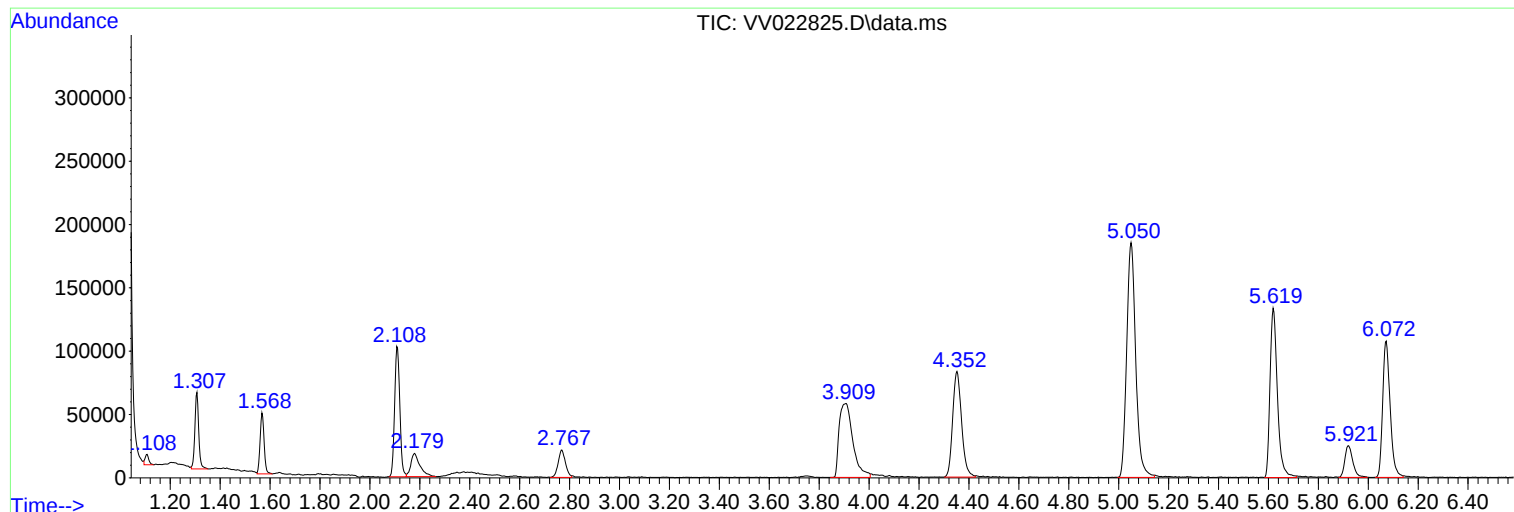

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022825.D
Acq On : 15 Oct 2021 04:39
Operator : SY/MD
Sample : M4223-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022825.D
Acq On : 15 Oct 2021 04:39
Operator : SY/MD
Sample : M4223-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
