

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
 Data File : VV022826.D
 Acq On : 15 Oct 2021 05:03
 Operator : SY/MD
 Sample : M4223-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGC7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	60520	62346	17.69%	2.153%
2	1.568	156	164	172	rBV	53088	58825	16.69%	2.031%
3	2.108	322	332	342	rBV	80582	119004	33.76%	4.110%
4	2.179	343	354	379	rVB	18353	46891	13.30%	1.619%
5	3.889	875	886	913	rBV2	34989	110819	31.44%	3.827%
6	4.352	1010	1030	1055	rBV2	64614	164249	46.60%	5.672%
7	5.050	1229	1247	1269	rBV2	141259	352457	100.00%	12.172%
8	5.619	1412	1424	1447	rBV	102885	211924	60.13%	7.319%
9	6.072	1552	1565	1582	rBV	81387	166327	47.19%	5.744%
10	6.989	1839	1850	1868	rBV	34274	62340	17.69%	2.153%
11	7.317	1939	1952	1971	rBV	169384	295720	83.90%	10.213%
12	7.397	1971	1977	1988	rVB	4766	8821	2.50%	0.305%
13	7.625	2040	2048	2064	rBV2	20700	35046	9.94%	1.210%
14	7.940	2137	2146	2151	rBV5	2405	4358	1.24%	0.151%
15	7.982	2151	2159	2170	rVB5	10770	18643	5.29%	0.644%
16	8.092	2183	2193	2217	rBV	155975	282759	80.23%	9.765%
17	8.854	2419	2430	2450	rBV	164539	267186	75.81%	9.227%
18	9.149	2513	2522	2528	rBV5	2183	3600	1.02%	0.124%
19	10.217	2842	2854	2878	rVB	58382	93136	26.42%	3.216%
20	10.381	2899	2905	2916	rVB3	4694	7233	2.05%	0.250%
21	11.249	3163	3175	3197	rBV	167294	257601	73.09%	8.896%
22	11.625	3279	3292	3312	rBV	164575	266360	75.57%	9.199%




Sum of corrected areas: 2895645

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022826.D
Acq On : 15 Oct 2021 05:03
Operator : SY/MD
Sample : M4223-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

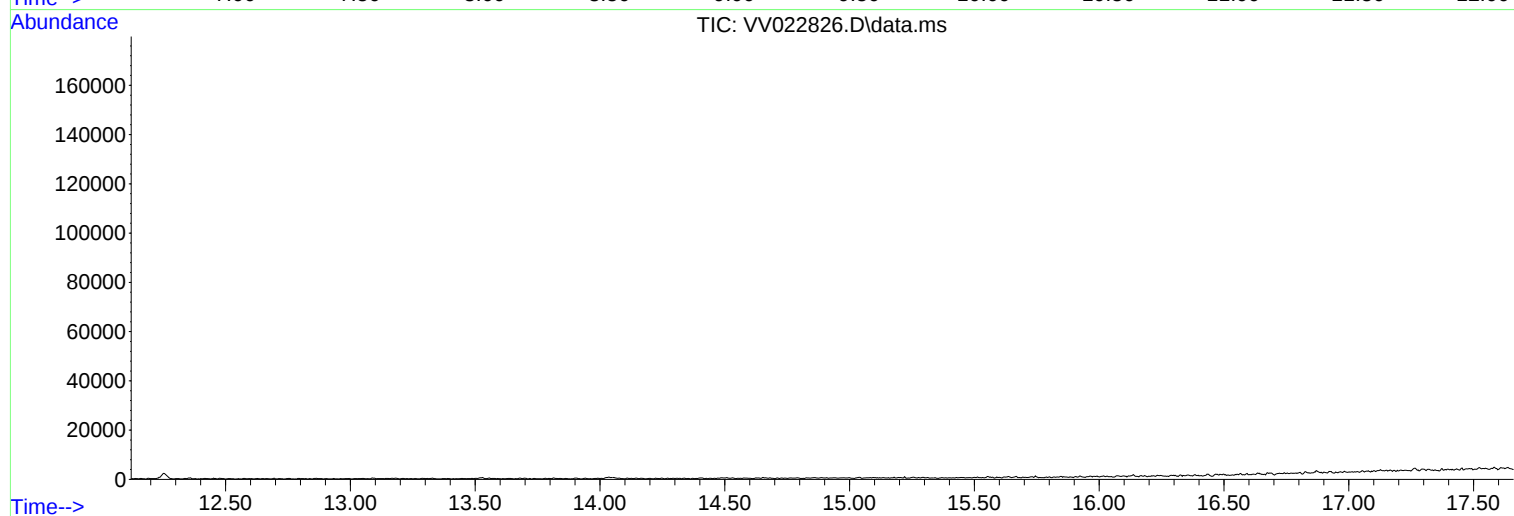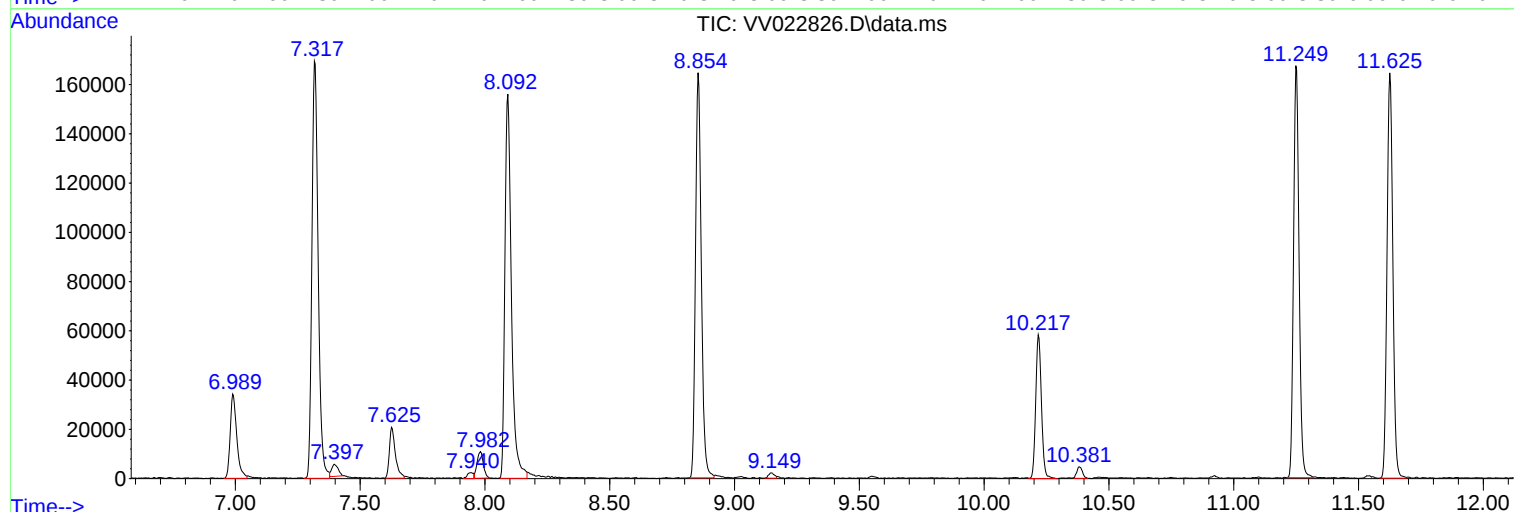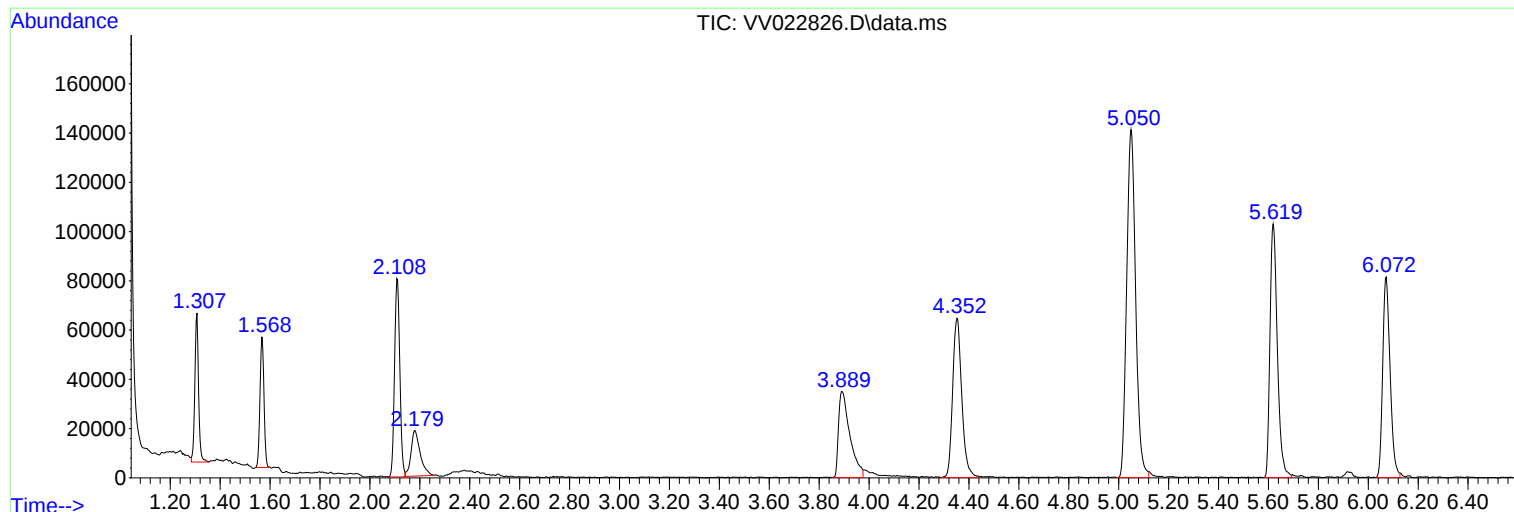

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022826.D
Acq On : 15 Oct 2021 05:03
Operator : SY/MD
Sample : M4223-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022826.D
Acq On : 15 Oct 2021 05:03
Operator : SY/MD
Sample : M4223-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
