


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101421\
Data File : VV022779.D
Acq On : 14 Oct 2021 09:10
Operator : SY/MD
Sample : BFB215
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB215

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 15 06:41:28 2021

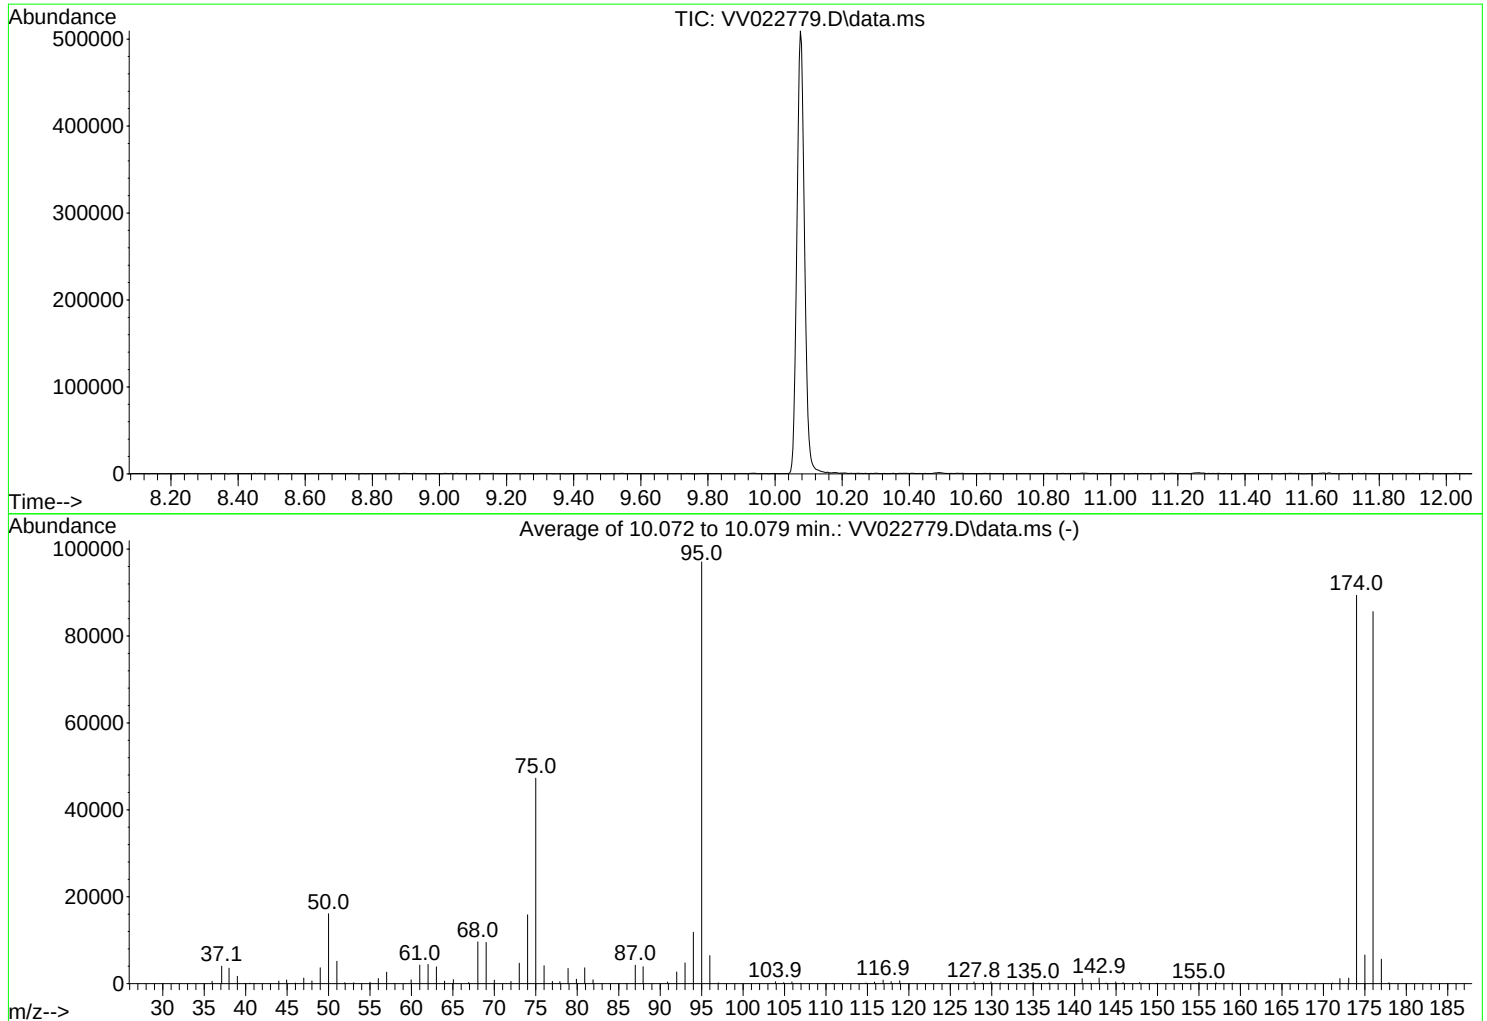

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	16084	PASS
75	95	30	80	48.7	47288	PASS
95	95	100	100	100.0	97072	PASS
96	95	5	9	6.6	6443	PASS
173	174	0.00	2	1.5	1297	PASS
174	95	50	120	92.1	89371	PASS
175	174	5	9	7.4	6591	PASS
176	174	95	105	95.8	85611	PASS
177	176	5	10	6.6	5628	PASS

m/z	Abundance
39.90	143.0
44.00	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
35.90	551.0
37.10	4024.0
38.00	3598.0
39.00	1524.0
40.00	185.0
44.00	776.0
44.90	907.0
46.00	173.0
47.00	1194.0
48.00	680.0
49.00	3515.0
50.00	15933.0
51.00	5097.0
52.00	180.0
53.10	218.0
55.00	324.0
56.00	1100.0
57.00	2555.0
57.90	134.0
59.90	840.0
61.00	4328.0
62.00	4372.0
63.00	3978.0
64.00	546.0
65.00	848.0
66.90	281.0
68.00	9472.0
69.00	9260.0
70.00	811.0
72.00	537.0
73.00	4554.0
74.00	15469.0
75.00	46920.0
76.00	4130.0
77.00	517.0
77.90	444.0
78.90	3381.0
79.90	914.0
80.90	3492.0
81.90	794.0
82.90	102.0
85.90	127.0
87.00	3968.0
87.90	3804.0
90.90	343.0
92.00	2512.0
93.00	4467.0
94.00	11797.0
95.00	94352.0
96.00	6446.0
97.10	185.0
103.90	423.0
104.90	256.0
105.90	380.0
107.00	107.0
114.80	150.0
115.90	370.0
116.90	821.0
117.90	464.0
118.90	661.0
127.80	341.0
128.90	144.0
129.90	355.0
131.00	144.0
135.00	264.0
136.90	193.0
140.90	963.0
141.90	140.0
142.90	1345.0
143.80	128.0
145.00	431.0
145.90	235.0
147.80	276.0
148.90	145.0
149.80	111.0
152.80	104.0
155.00	270.0
157.10	242.0
159.00	151.0
172.00	1234.0
173.00	1251.0
174.00	85176.0
175.00	6093.0
176.00	80576.0
177.00	5163.0
177.90	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
35.90	559.0
37.10	4130.0
38.00	3675.0
39.00	1765.0
39.90	166.0
40.50	137.0
40.90	120.0
44.00	800.0
44.90	881.0
46.00	168.0
47.00	1360.0
48.00	672.0
49.00	3798.0
50.00	16504.0
51.00	5346.0
52.00	219.0
53.10	220.0
54.00	123.0
55.00	362.0
56.00	1207.0
57.00	2761.0
57.90	114.0
59.90	951.0
61.00	4400.0
62.00	4569.0
63.00	3973.0
64.00	637.0
65.10	963.0
66.90	257.0
68.00	10038.0
69.00	9839.0
70.00	830.0
72.00	540.0
73.00	4921.0
74.00	16289.0
75.00	48600.0
76.00	4255.0
77.00	544.0
77.90	433.0
78.90	3614.0
79.90	1039.0
80.90	3782.0
81.90	920.0
87.00	4352.0
88.00	4069.0
90.90	382.0
92.00	2734.0
93.00	4942.0
94.00	12167.0
95.00	100320.0
96.00	6606.0
97.00	179.0
103.90	456.0
104.90	274.0
105.90	393.0
107.00	134.0
110.90	101.0
114.80	153.0
115.80	381.0
116.90	812.0
117.80	495.0
118.90	720.0
127.90	430.0
128.90	159.0
129.90	441.0
131.00	169.0
135.00	255.0
136.90	181.0
139.90	113.0
140.90	1174.0
141.90	162.0
143.00	1370.0
143.80	139.0
145.00	434.0
145.90	271.0
147.90	288.0
148.90	115.0
149.90	131.0
152.80	107.0
155.00	282.0
157.00	242.0
159.00	137.0
160.90	150.0
171.10	220.0
172.00	1158.0
173.00	1340.0
174.00	92240.0
175.00	6861.0
176.00	88520.0
177.00	5864.0
177.90	221.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
36.00	594.0
37.10	3902.0
38.00	3471.0
39.00	1809.0
39.90	176.0
40.50	169.0
40.90	114.0
44.00	752.0
45.00	782.0
46.00	147.0
47.00	1348.0
48.00	554.0
49.00	3615.0
50.00	15814.0
51.00	5038.0
51.90	257.0
53.00	195.0
54.00	142.0
55.00	315.0
56.00	1199.0
57.00	2624.0
60.00	909.0
61.00	4140.0
62.00	4297.0
63.00	3665.0
64.00	621.0
65.00	1000.0
66.90	249.0
68.00	9367.0
69.00	9412.0
70.00	799.0
72.00	486.0
73.00	4636.0
74.00	15789.0
75.00	46344.0
76.00	3987.0
77.00	518.0
77.90	416.0
78.90	3483.0
79.90	1127.0
80.90	3725.0
81.90	933.0
87.00	4391.0
88.00	3855.0
90.90	387.0
92.00	2791.0
93.00	4942.0
94.00	11459.0
95.00	96544.0
96.00	6276.0
97.00	158.0
103.90	437.0
104.90	234.0
105.90	418.0
106.90	137.0
110.80	127.0
114.80	144.0
115.80	374.0
116.90	788.0
117.80	455.0
118.90	661.0
127.90	473.0
128.90	154.0
129.90	428.0
131.10	185.0
135.00	253.0
136.90	188.0
139.90	121.0
140.90	1264.0
141.90	181.0
143.00	1219.0
143.80	146.0
144.90	395.0
145.80	239.0
147.90	288.0
150.00	122.0
152.80	101.0
155.00	258.0
157.00	244.0
159.00	120.0
160.90	160.0
171.10	211.0
172.00	1177.0
173.10	1299.0
174.00	90696.0
175.00	6819.0
176.00	87736.0
177.00	5856.0
177.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215