




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028553.D
 Acq On : 14 Oct 2022 17:14
 Operator : SY/MD
 Sample : VV1014WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Manual IntegrationsAPPROVED

Quant Time: Oct 15 02:41:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:40:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

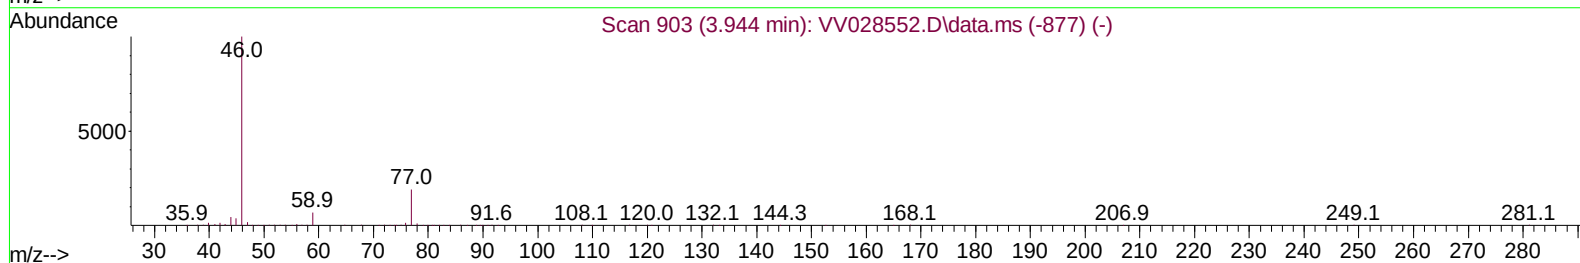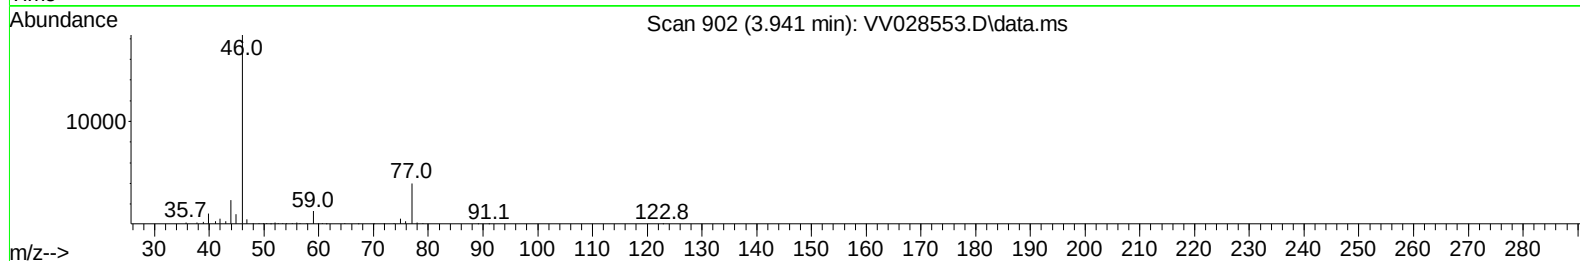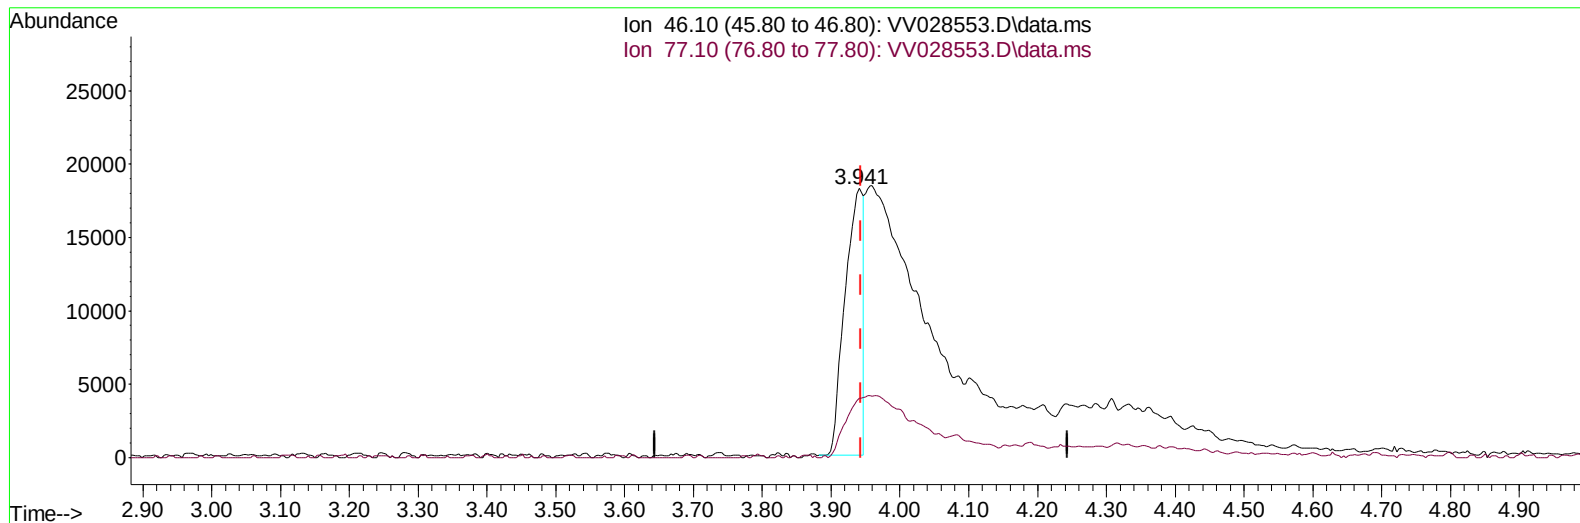

TIC: VV028553.D\data.ms

(20) 2-Butanone-d5 (S)

3.941min (-0.003) 8.26 ug/L

response 33772

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	20.40	65.59#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028553.D
Acq On : 14 Oct 2022 17:14
Operator : SY/MD
Sample : VV1014WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Manual IntegrationsAPPROVED

Quant Time: Oct 15 02:41:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 15 02:40:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
Supervised By :Mahesh Dadoda 10/18/2022

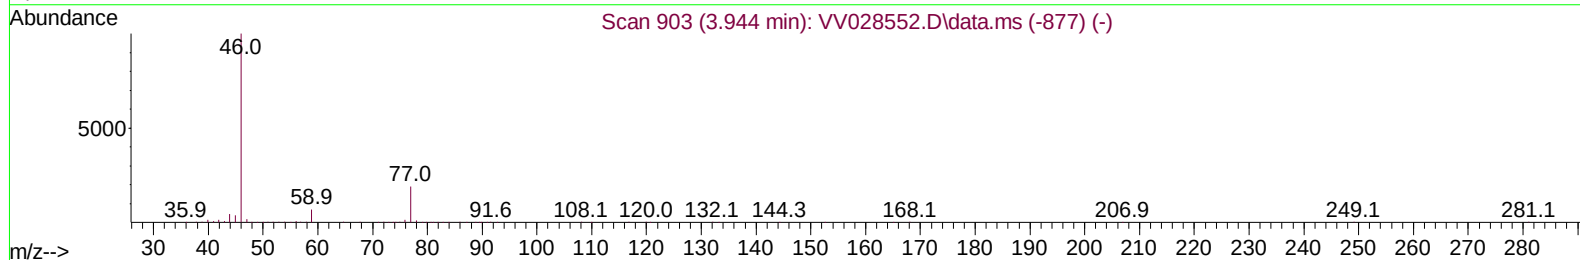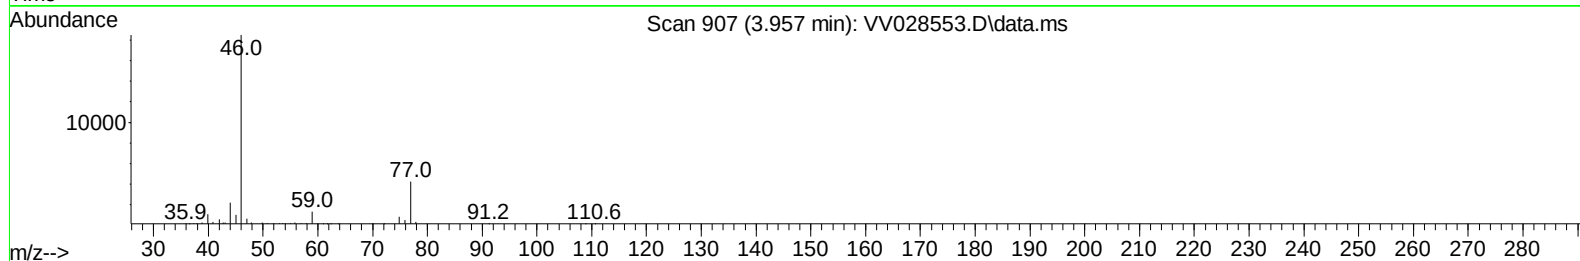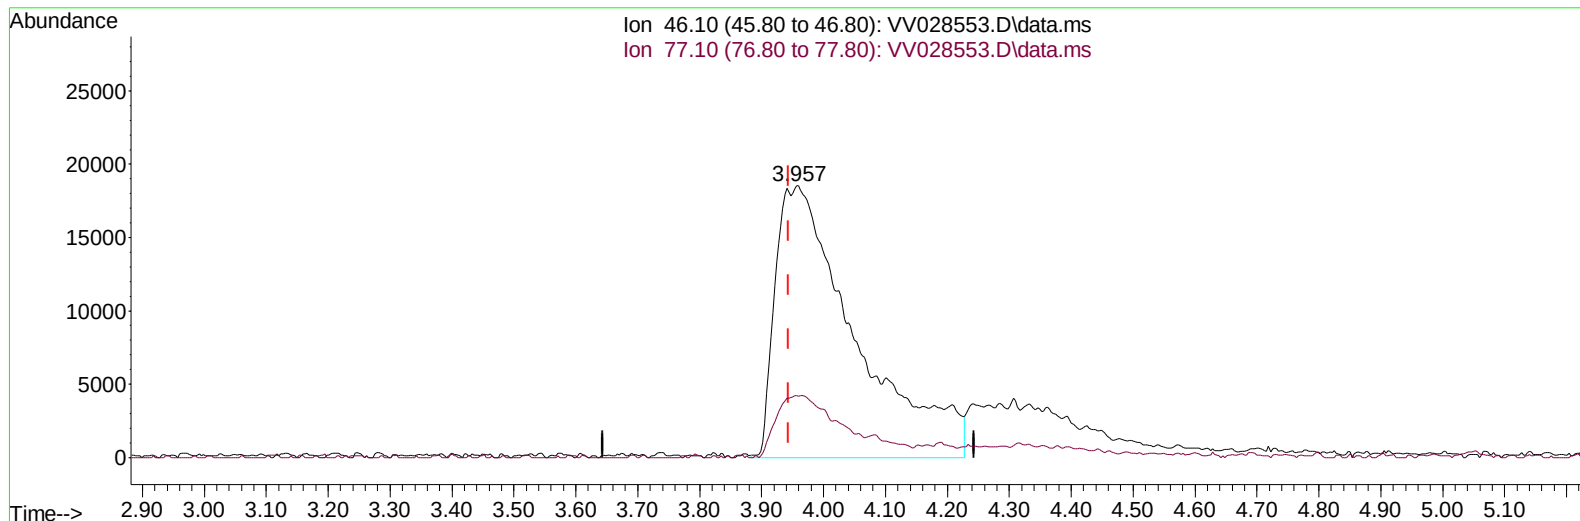

TIC: VV028553.D\data.ms

(20) 2-Butanone-d5 (S)

3.957min (+ 0.013) 40.63 ug/L m

response 166145

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	20.40	13.33#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028553.D
 Acq On : 14 Oct 2022 17:14
 Operator : SY/MD
 Sample : VV1014WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

Quant Time: Oct 15 02:41:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:40:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	221023	5.000	ug/L	0.01
28) Chlorobenzene-d5	8.847	117	206595	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	93936	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	95223	5.006	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 100.200%			
7) Chloroethane-d5	1.564	69	82131	5.252	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 105.000%			
11) 1,1-Dichloroethene-d2	2.105	63	130545	3.789	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 75.800%			
20) 2-Butanone-d5	3.957	46	166145m	40.630	ug/L	0.01
Spiked Amount 50.000	Range 40 - 130		Recovery = 81.260%			
24) Chloroform-d	4.342	84	136894	4.700	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 94.000%			
26) 1,2-Dichloroethane-d4	5.031	65	73808	4.862	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 97.200%			
32) Benzene-d6	5.047	84	293653	4.402	ug/L	0.02
Spiked Amount 5.000	Range 70 - 125		Recovery = 88.000%			
36) 1,2-Dichloropropane-d6	6.066	67	97191	4.515	ug/L	0.01
Spiked Amount 5.000	Range 60 - 140		Recovery = 90.200%			
41) Toluene-d8	7.310	98	246614	4.666	ug/L	0.02
Spiked Amount 5.000	Range 70 - 130		Recovery = 93.400%			
43) trans-1,3-Dichloroprop...	7.619	79	31831	4.377	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 87.600%			
46) 2-Hexanone-d5	8.092	63	151556	48.284	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 96.560%			
56) 1,1,2,2-Tetrachloroeth...	10.207	84	61301	4.782	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 95.600%			
66) 1,2-Dichlorobenzene-d4	11.616	152	78822	5.085	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 101.800%			
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	6122	0.316	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028553.D
Acq On : 14 Oct 2022 17:14
Operator : SY/MD
Sample : VV1014WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Manual IntegrationsAPPROVED

Quant Time: Oct 15 02:41:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 15 02:40:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
Supervised By :Mahesh Dadoda 10/18/2022

