




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028562.D
 Acq On : 14 Oct 2022 20:49
 Operator : SY/MD
 Sample : N5103-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BX1

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:00:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

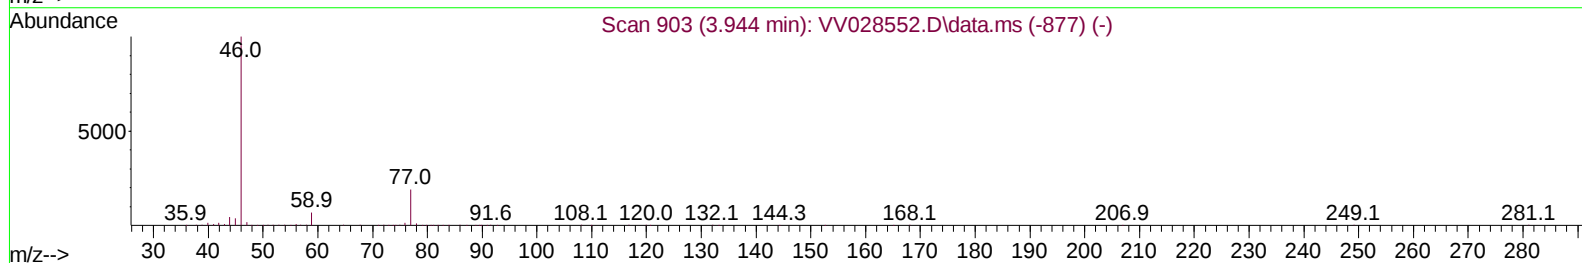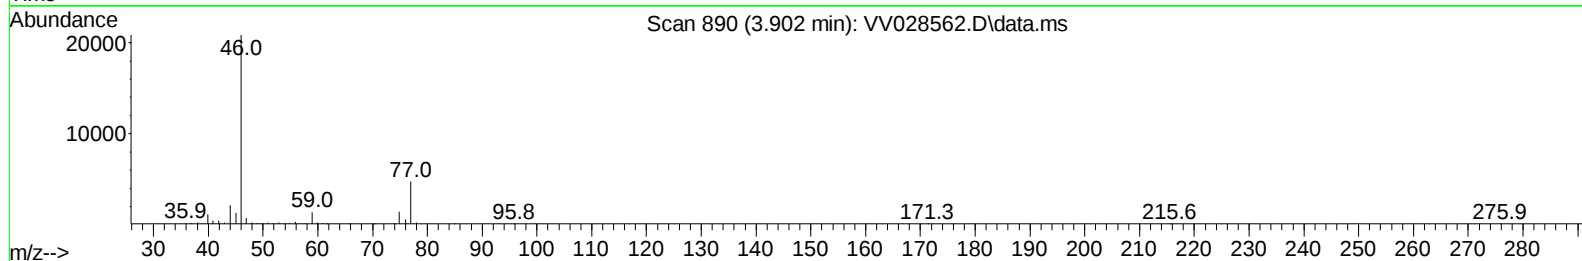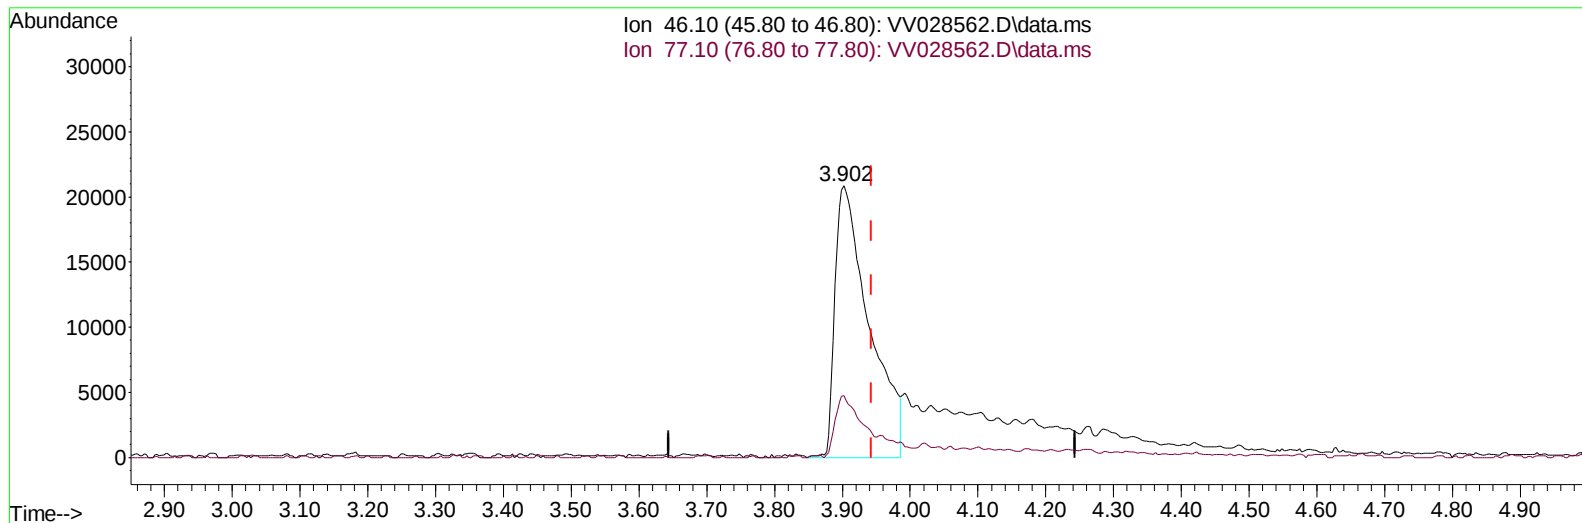

TIC: VV028562.D\data.ms

(20) 2-Butanone-d5 (S)

3.902min (-0.042) 19.65 ug/L

response 73270

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	20.40	17.54
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028562.D
 Acq On : 14 Oct 2022 20:49
 Operator : SY/MD
 Sample : N5103-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BX1

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:00:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

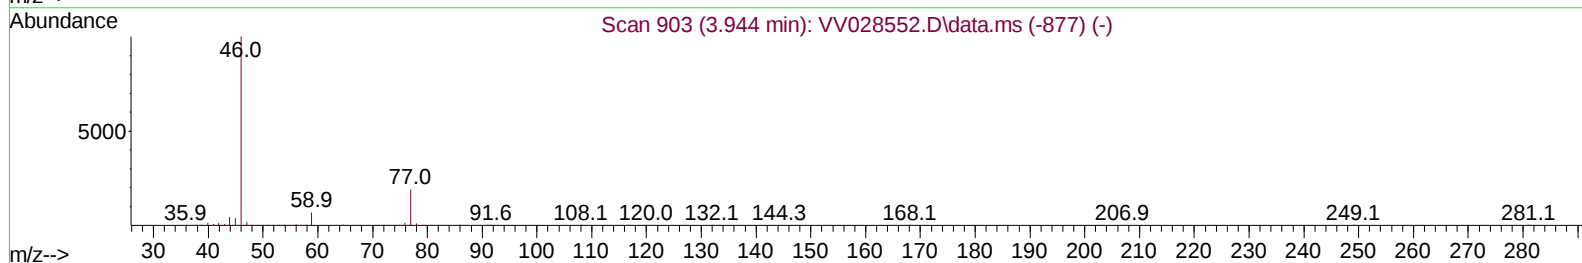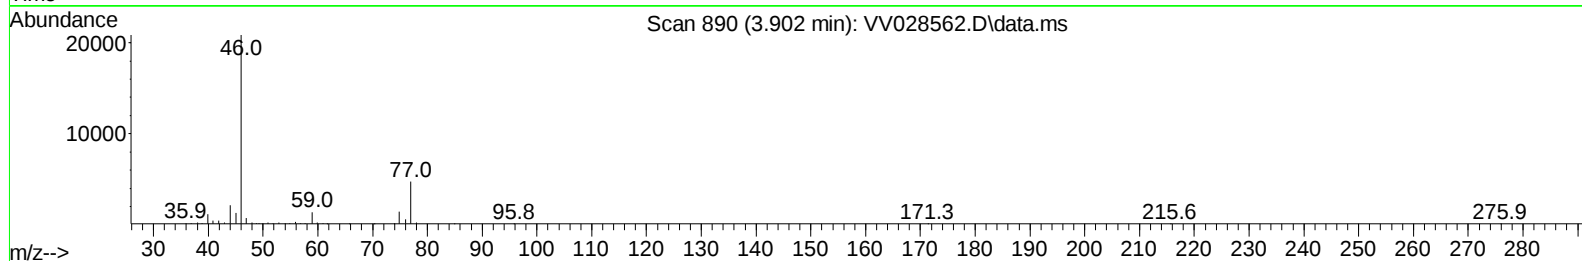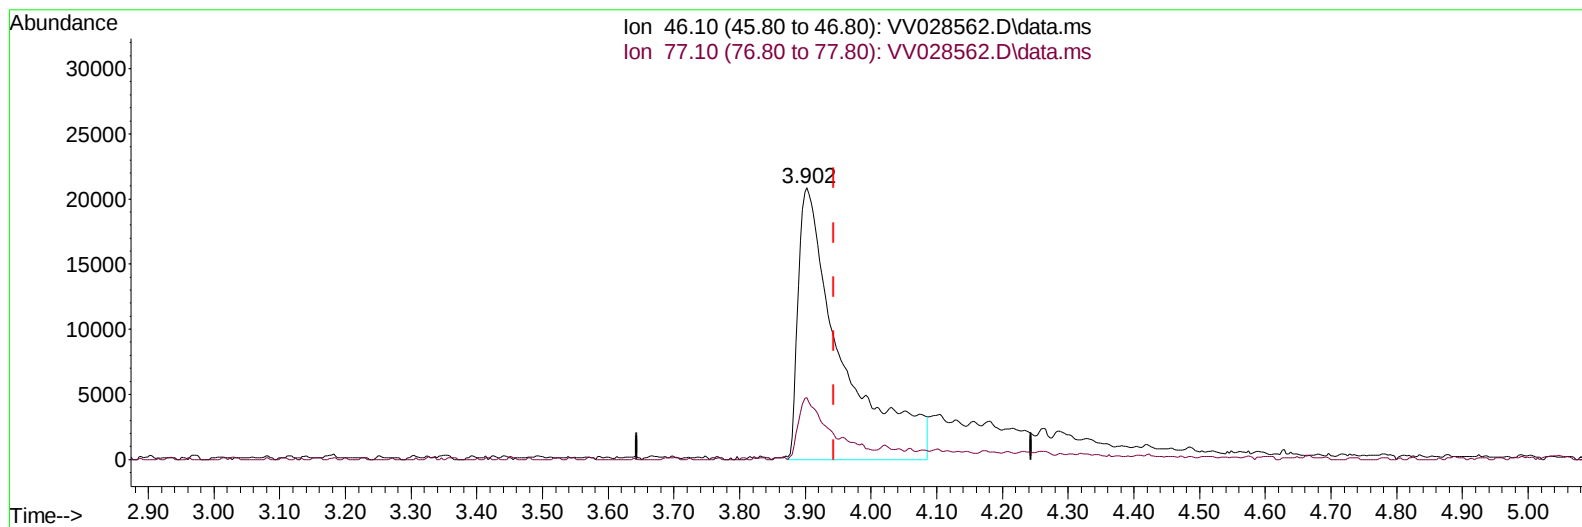

TIC: VV028562.D\data.ms

(20) 2-Butanone-d5 (S)

3.902min (-0.042) 25.63 ug/L m

response 95574

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	20.40	13.45#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028562.D
 Acq On : 14 Oct 2022 20:49
 Operator : SY/MD
 Sample : N5103-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBX1

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:00:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		201515	5.000	ug/L	0.02
28) Chlorobenzene-d5	8.847	117		186089	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152		83977	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		90706	5.230	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.600%	
7) Chloroethane-d5	1.565	69		71647	5.025	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.600%	
11) 1,1-Dichloroethene-d2	2.105	63		121851	3.879	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.600%	
20) 2-Butanone-d5	3.902	46		95574m	25.635	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	51.260%	
24) Chloroform-d	4.346	84		111432	4.196	ug/L	0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%	
26) 1,2-Dichloroethane-d4	5.031	65		54275	3.921	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.400%	
32) Benzene-d6	5.047	84		241368	4.017	ug/L	0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.400%	
36) 1,2-Dichloropropane-d6	6.066	67		75541	3.896	ug/L	0.01
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.000%	
41) Toluene-d8	7.314	98		204762	4.301	ug/L	0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%	
43) trans-1,3-Dichloroprop...	7.622	79		18022	2.751	ug/L	0.01
Spiked Amount	5.000	Range	55 - 130	Recovery	=	55.000%	
46) 2-Hexanone-d5	8.088	63		88463	31.289	ug/L	-0.01
Spiked Amount	50.000	Range	45 - 130	Recovery	=	62.580%	
56) 1,1,2,2-Tetrachloroeth...	10.211	84		43310	3.751	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.000%	
66) 1,2-Dichlorobenzene-d4	11.616	152		58426	4.216	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.400%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028562.D
Acq On : 14 Oct 2022 20:49
Operator : SY/MD
Sample : N5103-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BX1

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:00:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 15 02:57:21 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
Supervised By :Mahesh Dadoda 10/18/2022

