




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028565.D
 Acq On : 14 Oct 2022 22:00
 Operator : SY/MD
 Sample : N5103-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B93

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:01:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

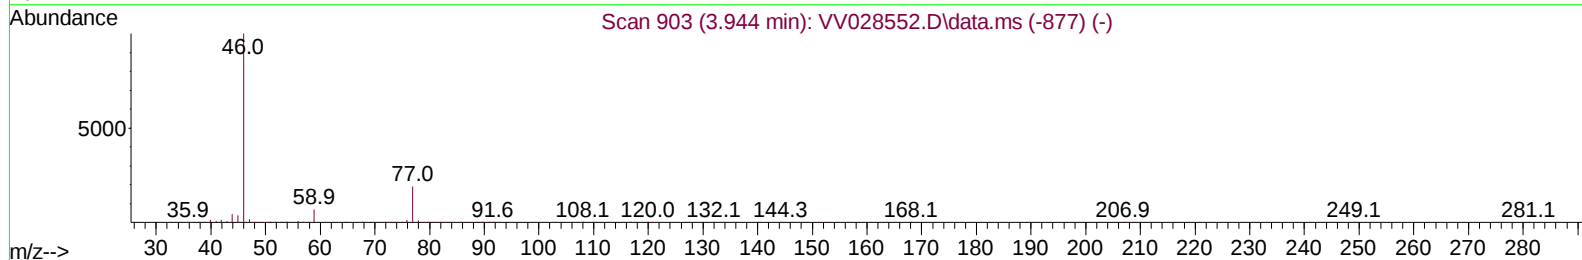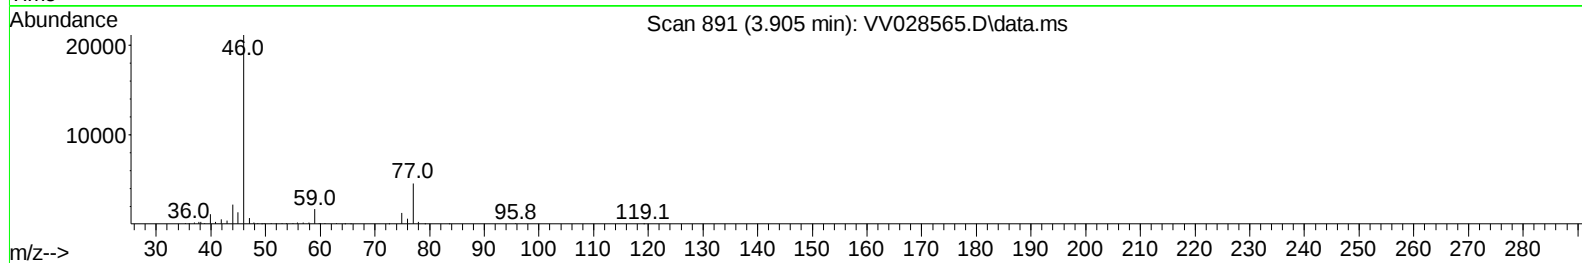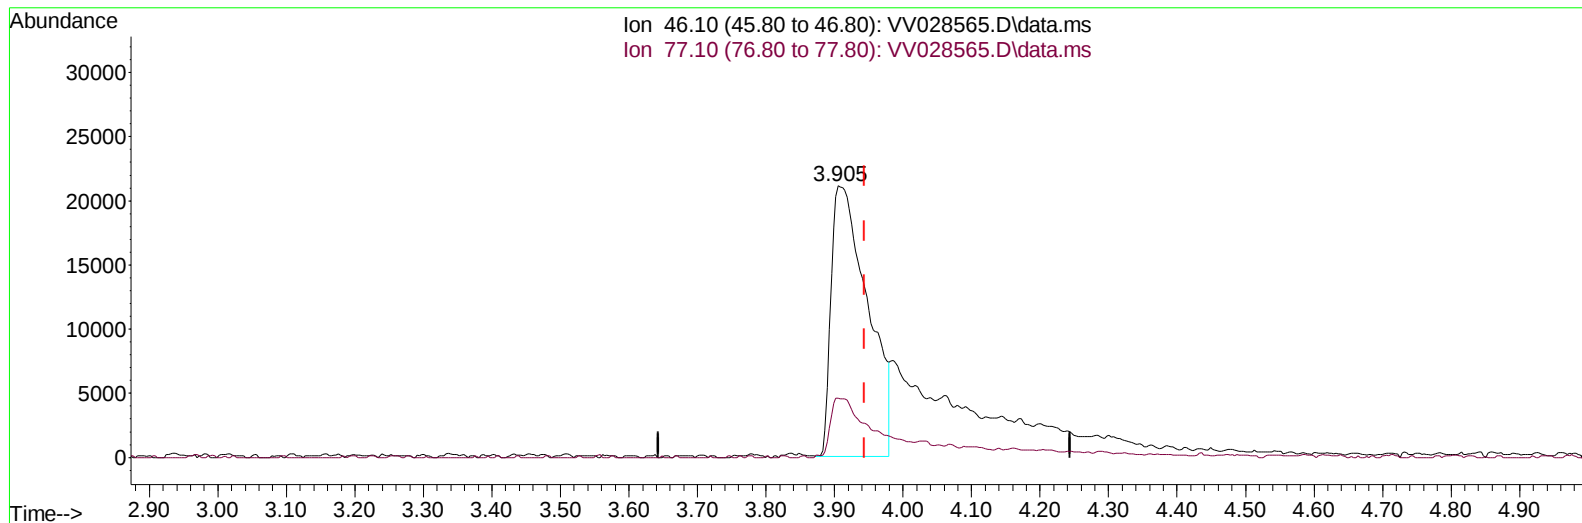

TIC: VV028565.D\data.ms

(20) 2-Butanone-d5 (S)

3.905min (-0.038) 20.84 ug/L

response 77935

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	20.40	25.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028565.D
 Acq On : 14 Oct 2022 22:00
 Operator : SY/MD
 Sample : N5103-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B93

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:01:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

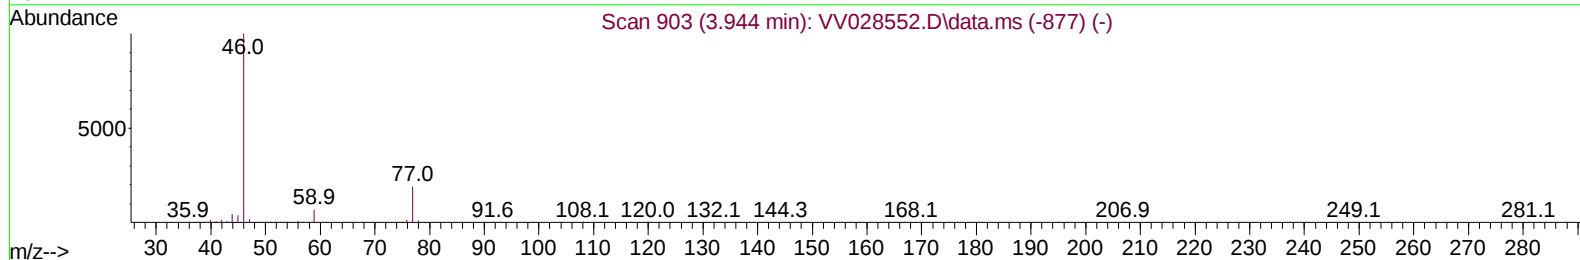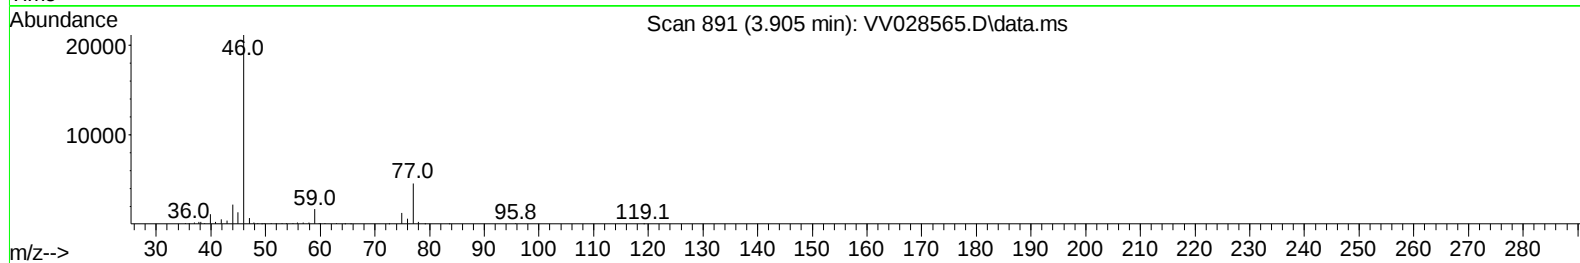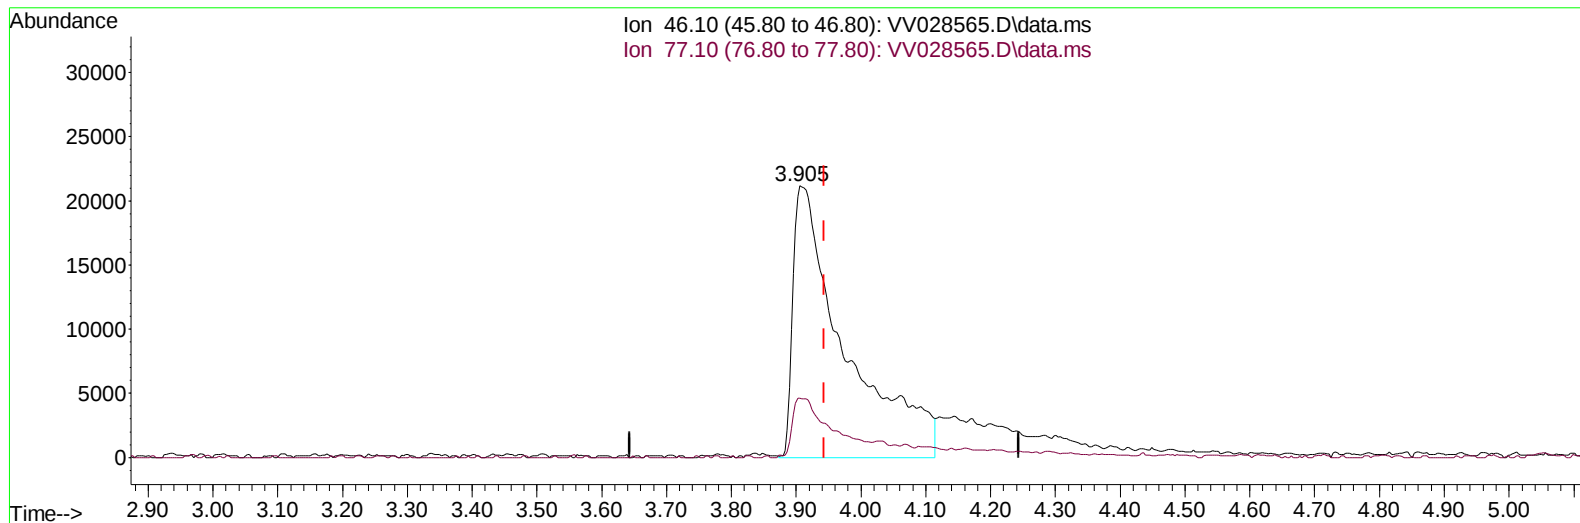

TIC: VV028565.D\data.ms

(20) 2-Butanone-d5 (S)

3.905min (-0.038) 31.53 ug/L m

response 117919

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	20.40	16.76
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028565.D
 Acq On : 14 Oct 2022 22:00
 Operator : SY/MD
 Sample : N5103-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B93

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:01:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	202121	5.000	ug/L	0.02
28) Chlorobenzene-d5	8.847	117	187850	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	85187	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	89234	5.130	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	102.600%	
7) Chloroethane-d5	1.565	69	69476	4.858	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	97.200%	
11) 1,1-Dichloroethene-d2	2.105	63	118566	3.763	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	75.200%	
20) 2-Butanone-d5	3.905	46	117919m	31.533	ug/L	-0.04
Spiked Amount 50.000	Range 40	- 130	Recovery	=	63.060%	
24) Chloroform-d	4.346	84	107231	4.026	ug/L	0.01
Spiked Amount 5.000	Range 70	- 125	Recovery	=	80.600%	
26) 1,2-Dichloroethane-d4	5.031	65	55769	4.017	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	80.400%	
32) Benzene-d6	5.047	84	231869	3.823	ug/L	0.02
Spiked Amount 5.000	Range 70	- 125	Recovery	=	76.400%	
36) 1,2-Dichloropropane-d6	6.066	67	75362	3.850	ug/L	0.01
Spiked Amount 5.000	Range 60	- 140	Recovery	=	77.000%	
41) Toluene-d8	7.313	98	198158	4.123	ug/L	0.02
Spiked Amount 5.000	Range 70	- 130	Recovery	=	82.400%	
43) trans-1,3-Dichloroprop...	7.622	79	18373	2.778	ug/L	0.01
Spiked Amount 5.000	Range 55	- 130	Recovery	=	55.600%	
46) 2-Hexanone-d5	8.088	63	101996	35.737	ug/L	-0.01
Spiked Amount 50.000	Range 45	- 130	Recovery	=	71.480%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	44851	3.848	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	77.000%	
66) 1,2-Dichlorobenzene-d4	11.616	152	59051	4.201	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	84.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028565.D
Acq On : 14 Oct 2022 22:00
Operator : SY/MD
Sample : N5103-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0B93

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:01:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 15 02:57:21 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
Supervised By :Mahesh Dadoda 10/18/2022

