




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028567.D
 Acq On : 14 Oct 2022 22:48
 Operator : SY/MD
 Sample : N5103-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BB3

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:01:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

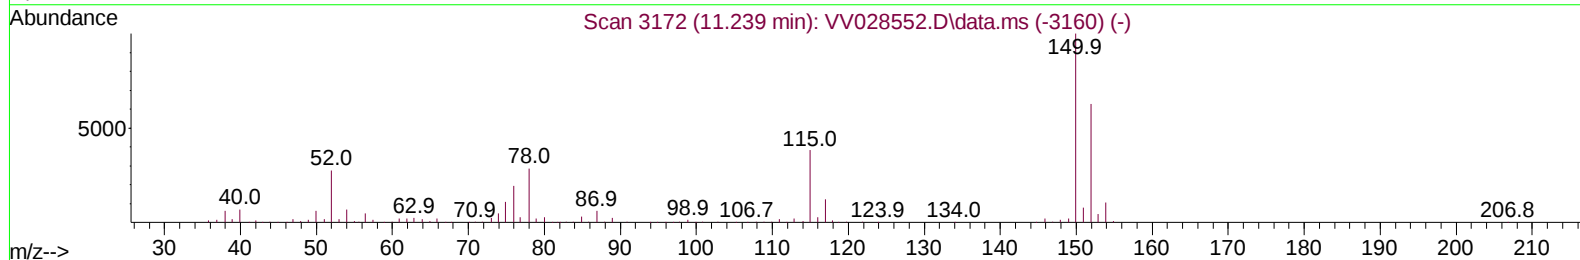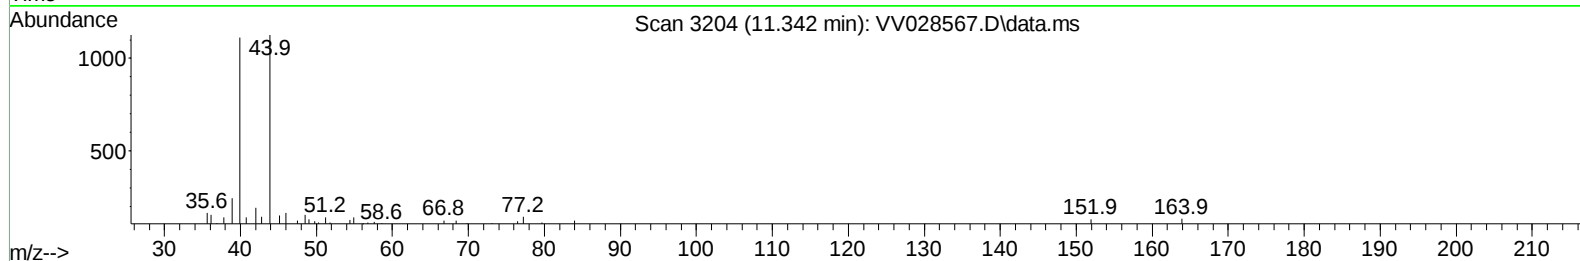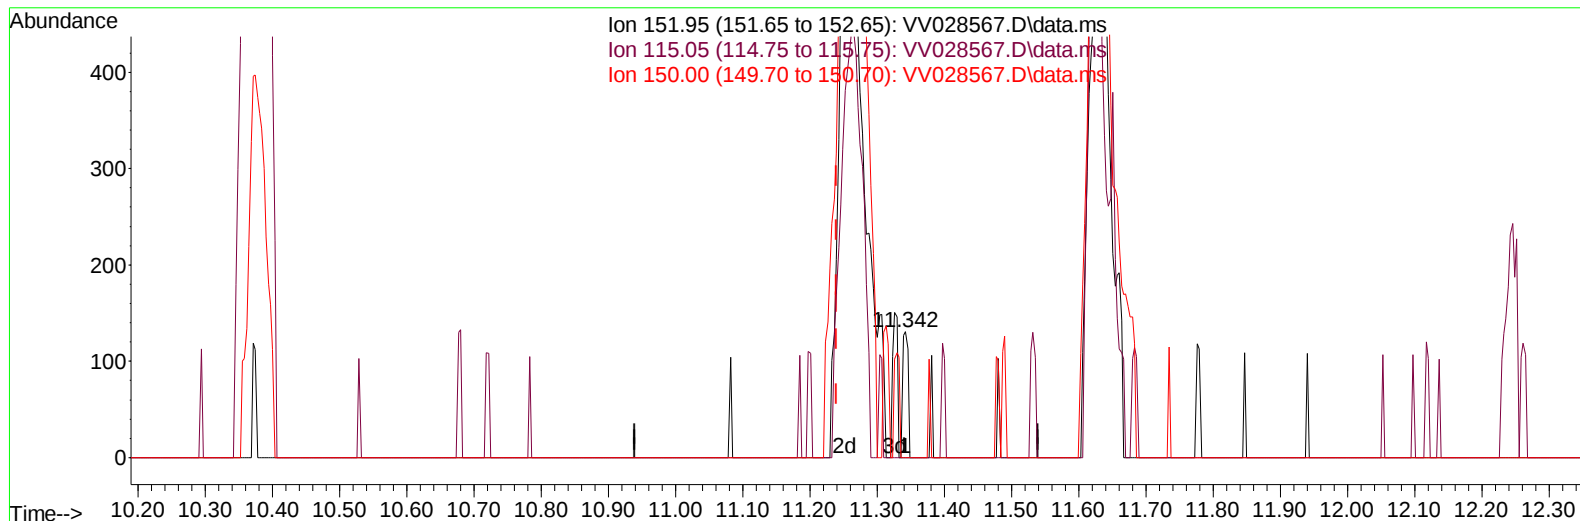

TIC: VV028567.D\data.ms

(58) 1,4-Dichlorobenzene-d4 (I)

11.342min (+ 0.103) 5.00 ug/L

response 72

Ion	Exp%	Act%
151.95	100.00	100.00
115.05	61.50	59.72
150.00	170.80	55.56
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028567.D
Acq On : 14 Oct 2022 22:48
Operator : SY/MD
Sample : N5103-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 10/17/2022
Supervised By :Mahesh Dadoda 10/18/2022

Quant Time: Oct 15 03:01:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 15 02:57:21 2022
Response via : Initial Calibration

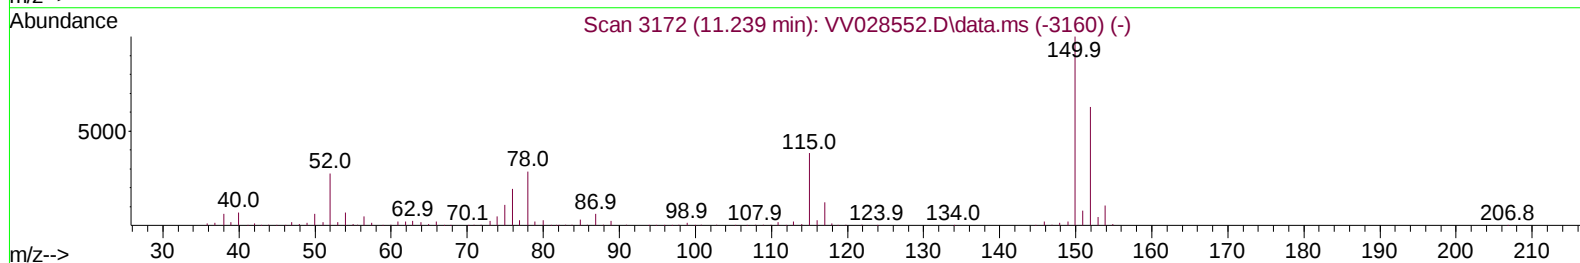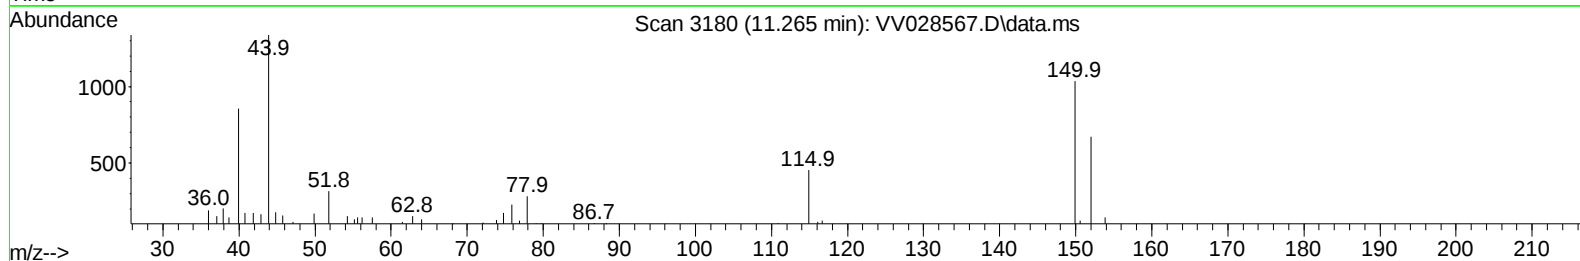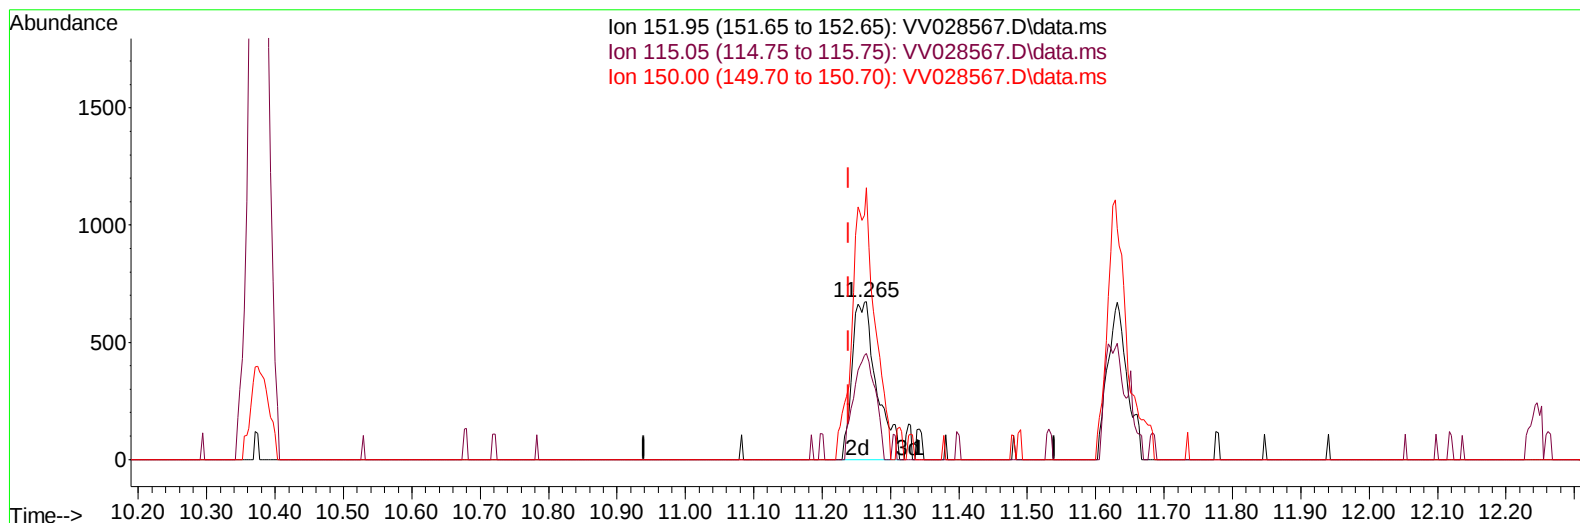

TIC: VV028567.D\data.ms

(58) 1,4-Dichlorobenzene-d4 (I)

11.265min (+ 0.026) 5.00 ug/L m

response 1676

Ion	Exp%	Act%
151.95	100.00	100.00
115.05	61.50	2.57
150.00	170.80	2.39
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028567.D
 Acq On : 14 Oct 2022 22:48
 Operator : SY/MD
 Sample : N5103-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBB3

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:01:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.635	114	5053	5.000	ug/L	# 0.03
28) Chlorobenzene-d5	8.863	117	2222	5.000	ug/L	# 0.02
58) 1,4-Dichlorobenzene-d4	11.265	152	1676m	5.000	ug/L	0.03
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	14959	34.399	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	= 688.000%	#	
7) Chloroethane-d5	1.568	69	8991	25.149	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	= 503.000%	#	
11) 1,1-Dichloroethene-d2	2.105	63	12975	16.473	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	= 329.400%	#	
20) 2-Butanone-d5	3.905	46	53928	576.843	ug/L	-0.04
Spiked Amount 50.000	Range 40	- 130	Recovery	= 1153.680%	#	
24) Chloroform-d	4.352	84	6685	10.039	ug/L	0.02
Spiked Amount 5.000	Range 70	- 125	Recovery	= 200.800%	#	
26) 1,2-Dichloroethane-d4	5.056	65	4061	11.701	ug/L	0.04
Spiked Amount 5.000	Range 70	- 130	Recovery	= 234.000%	#	
32) Benzene-d6	5.059	84	10025	13.973	ug/L	0.03
Spiked Amount 5.000	Range 70	- 125	Recovery	= 279.400%	#	
36) 1,2-Dichloropropane-d6	6.079	67	3751	16.201	ug/L	0.03
Spiked Amount 5.000	Range 60	- 140	Recovery	= 324.000%	#	
41) Toluene-d8	7.333	98	3315	5.832	ug/L	0.04
Spiked Amount 5.000	Range 70	- 130	Recovery	= 116.600%		
43) trans-1,3-Dichloroprop...	0.000	79	0d	0.000	ug/L	
Spiked Amount 5.000	Range 55	- 130	Recovery	= 0.000%	#	
46) 2-Hexanone-d5	8.098	63	20602	610.259	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	= 1220.520%	#	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	3858	27.981	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	= 559.600%	#	
66) 1,2-Dichlorobenzene-d4	11.631	152	1335	4.827	ug/L	0.02
Spiked Amount 5.000	Range 80	- 120	Recovery	= 96.600%		
Target Compounds						
						Qvalue
13) Acetone	2.178	43	8894	135.478	ug/L	82
16) Methylene chloride	2.506	84	3524	7.952	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028567.D
Acq On : 14 Oct 2022 22:48
Operator : SY/MD
Sample : N5103-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB3

Manual IntegrationsAPPROVED

Quant Time: Oct 15 03:01:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 15 02:57:21 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
Supervised By :Mahesh Dadoda 10/18/2022

