

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101422\
 Data File : VW028568.D
 Acq On : 14 Oct 2022 23:12
 Operator : SY/MD
 Sample : N5103-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBX0

Quant Time: Oct 15 03:02:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	203794	5.000	ug/L	0.02
28) Chlorobenzene-d5	8.847	117	191446	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	85717	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	86916	4.956	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.200%
7) Chloroethane-d5	1.565	69	72073	4.998	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.000%
11) 1,1-Dichloroethene-d2	2.105	63	119625	3.766	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.400%
20) 2-Butanone-d5	3.899	46	146048	38.734	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.460%
24) Chloroform-d	4.346	84	112721	4.197	ug/L	0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
26) 1,2-Dichloroethane-d4	5.031	65	59616	4.259	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
32) Benzene-d6	5.047	84	239170	3.869	ug/L	0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.400%
36) 1,2-Dichloropropane-d6	6.066	67	77894	3.905	ug/L	0.01
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.000%
41) Toluene-d8	7.314	98	203166	4.148	ug/L	0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.000%
43) trans-1,3-Dichloroprop...	7.625	79	19800	2.938	ug/L	0.02
Spiked Amount	5.000	Range	55 - 130	Recovery	=	58.800%
46) 2-Hexanone-d5	8.088	63	106469	36.604	ug/L	-0.01
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.200%
56) 1,1,2,2-Tetrachloroeth...	10.211	84	47921	4.034	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.600%
66) 1,2-Dichlorobenzene-d4	11.619	152	59712	4.222	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.400%
Target Compounds						
13) Acetone	2.188	43	11508	4.346	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028568.D
Acq On : 14 Oct 2022 23:12
Operator : SY/MD
Sample : N5103-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BX0

Quant Time: Oct 15 03:02:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 15 02:57:21 2022
Response via : Initial Calibration

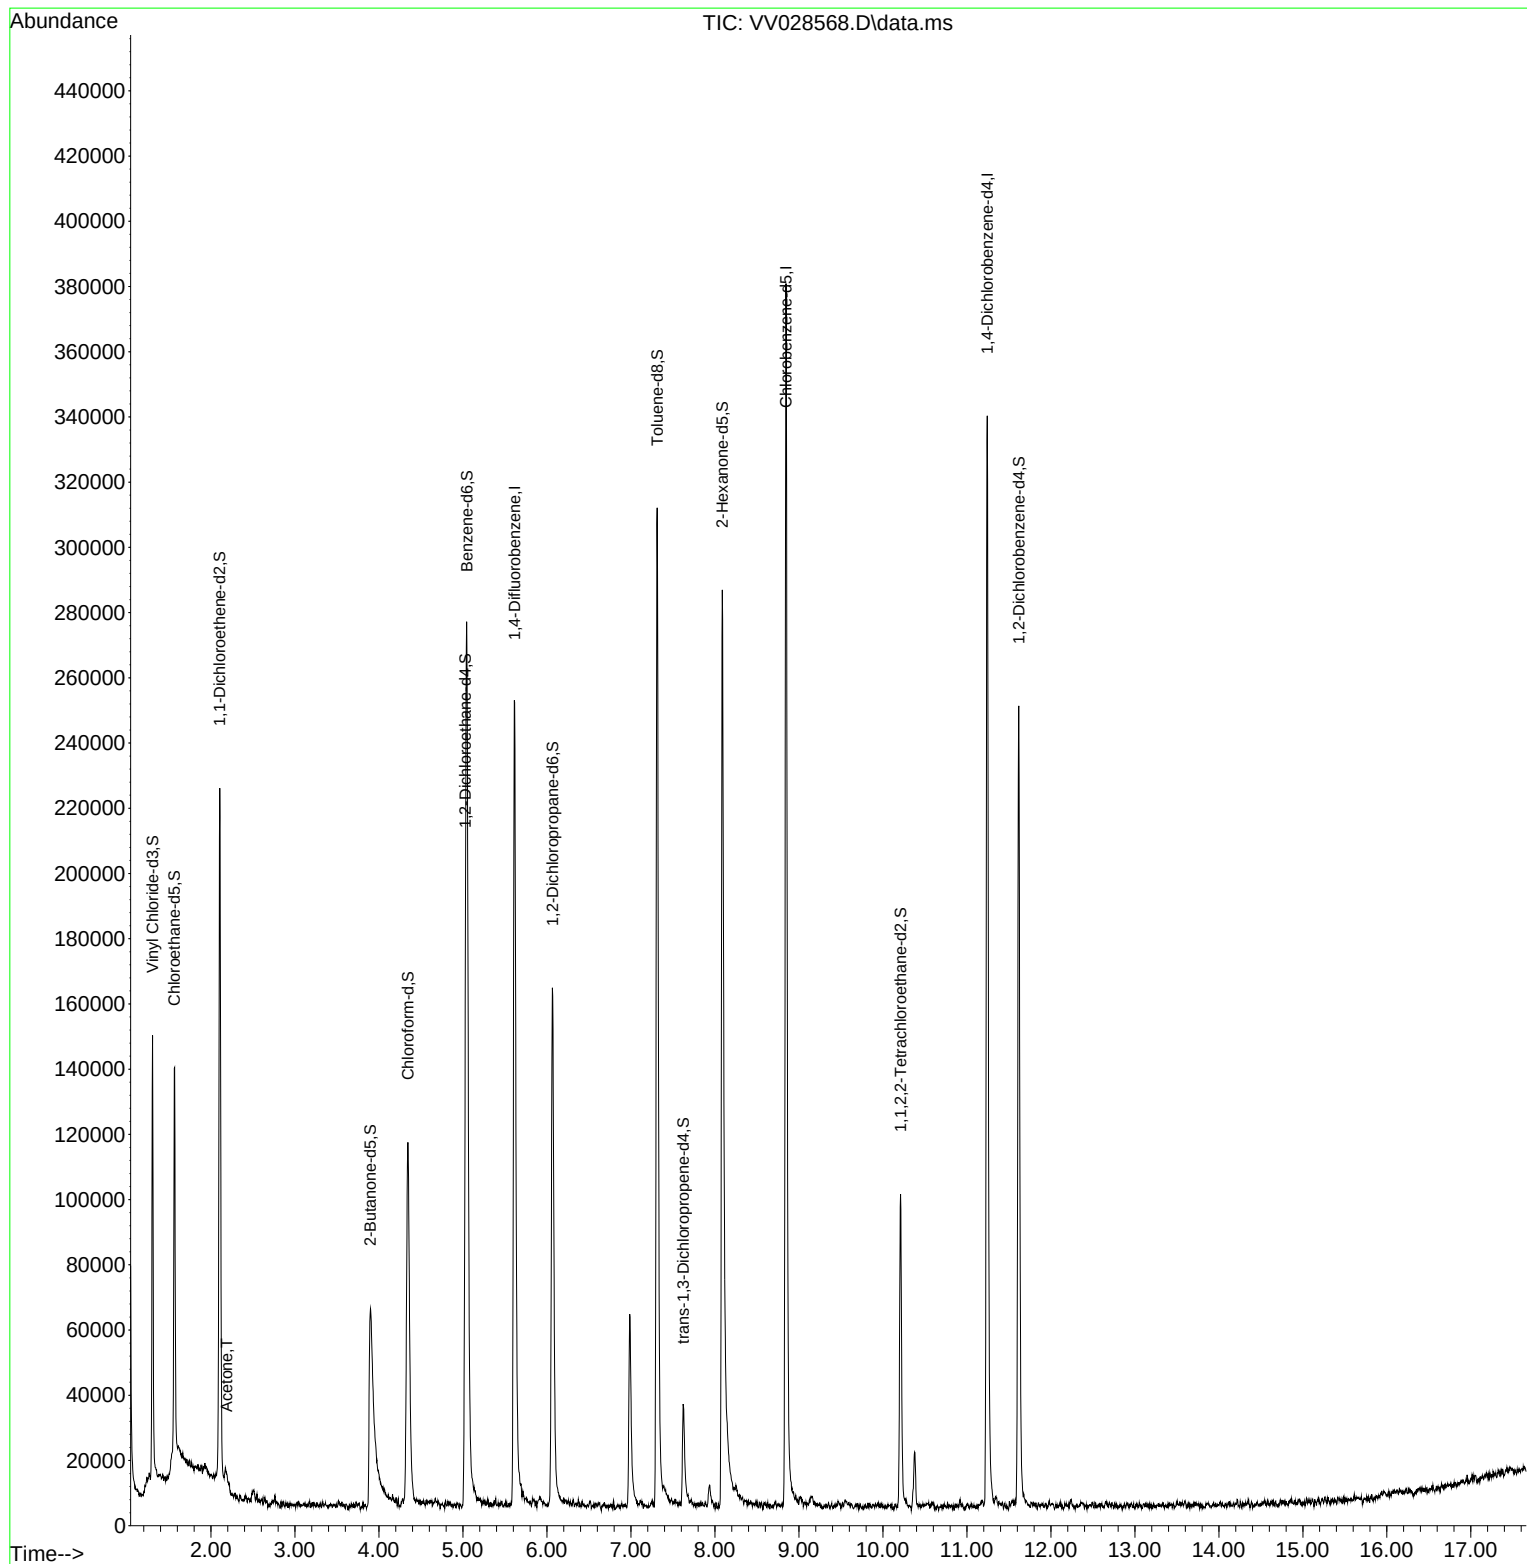

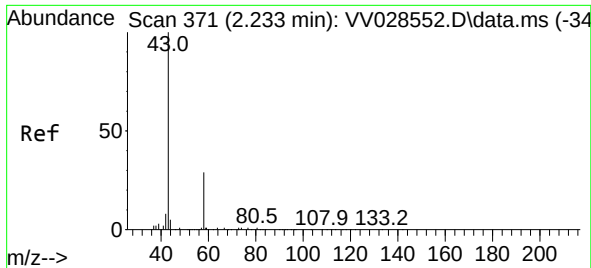

#13
 Acetone
 Concen: 4.346 ug/L
 RT: 2.188 min Scan# 31
 Delta R.T. -0.045 min
 Lab File: VV028568.D
 Acq: 14 Oct 2022 23:12

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BX0

Tgt Ion: 43 Resp: 11508
 Ion Ratio Lower Upper
 43 100
 58 30.3 0.0 48.6

