

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028569.D
 Acq On : 14 Oct 2022 23:36
 Operator : SY/MD
 Sample : N5103-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B99

Quant Time: Oct 15 03:02:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	192668	5.000	ug/L	0.02
28) Chlorobenzene-d5	8.847	117	175489	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	74978	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	86545	5.219	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	104.400%	
7) Chloroethane-d5	1.564	69	69674	5.111	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	102.200%	
11) 1,1-Dichloroethene-d2	2.105	63	113160	3.768	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	75.400%	
20) 2-Butanone-d5	3.902	46	132577	37.192	ug/L	-0.04
Spiked Amount	50.000	Range 40 - 130	Recovery	=	74.380%	
24) Chloroform-d	4.342	84	110890	4.367	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.400%	
26) 1,2-Dichloroethane-d4	5.031	65	58598	4.428	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.600%	
32) Benzene-d6	5.047	84	233686	4.124	ug/L	0.02
Spiked Amount	5.000	Range 70 - 125	Recovery	=	82.400%	
36) 1,2-Dichloropropane-d6	6.066	67	76599	4.189	ug/L	0.01
Spiked Amount	5.000	Range 60 - 140	Recovery	=	83.800%	
41) Toluene-d8	7.313	98	189401	4.219	ug/L	0.02
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.400%	
43) trans-1,3-Dichloroprop...	7.625	79	18922	3.063	ug/L	0.02
Spiked Amount	5.000	Range 55 - 130	Recovery	=	61.200%	
46) 2-Hexanone-d5	8.088	63	100160	37.566	ug/L	-0.01
Spiked Amount	50.000	Range 45 - 130	Recovery	=	75.140%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	45739	4.200	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	84.000%	
66) 1,2-Dichlorobenzene-d4	11.619	152	55341	4.473	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	89.400%	
Target Compounds					Qvalue	
13) Acetone	2.191	43	9745	3.893	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028569.D
Acq On : 14 Oct 2022 23:36
Operator : SY/MD
Sample : N5103-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B99

Quant Time: Oct 15 03:02:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 15 02:57:21 2022
Response via : Initial Calibration

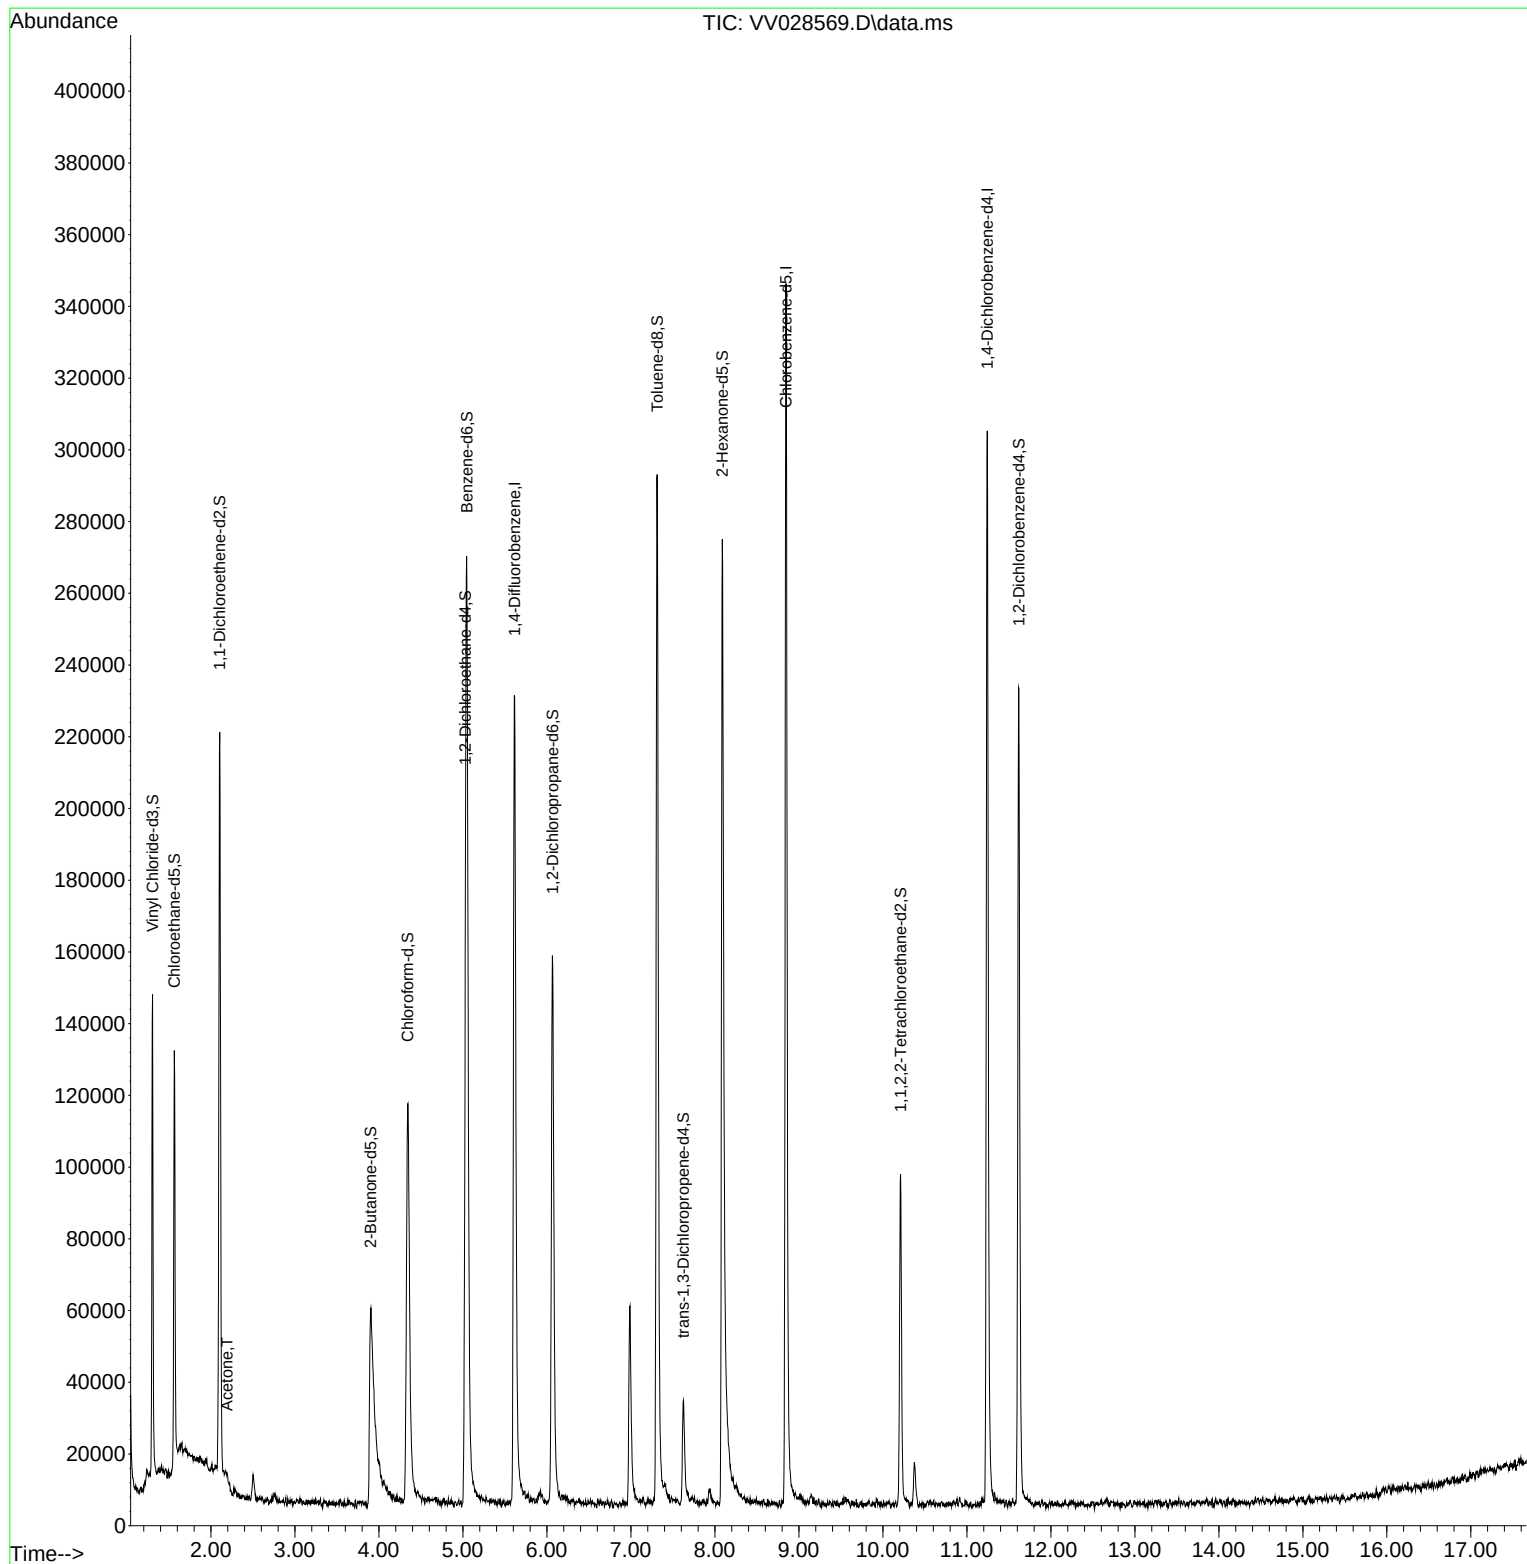

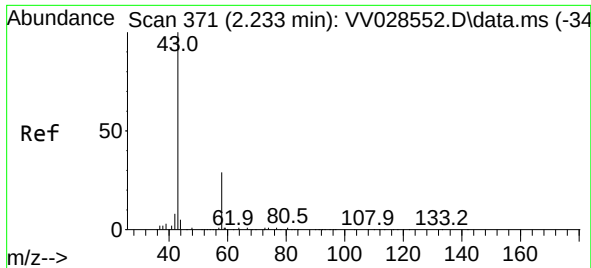

#13

Acetone

Concen: 3.893 ug/L

RT: 2.191 min Scan# 31

Delta R.T. -0.042 min

Lab File: VV028569.D

Acq: 14 Oct 2022 23:36

Instrument :

MSVOA_V

ClientSampleId :

C0B99

Tgt Ion: 43 Resp: 9745

Ion Ratio Lower Upper

43 100

58 32.6 0.0 48.6

