

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101422\
 Data File : VW028570.D
 Acq On : 15 Oct 2022 00:00
 Operator : SY/MD
 Sample : N5060-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1BC3

Quant Time: Oct 15 03:02:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 15 02:57:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	191108	5.000	ug/L	0.02
28) Chlorobenzene-d5	8.847	117	176585	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	77349	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	80165	4.874	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.400%
7) Chloroethane-d5	1.568	69	66572	4.923	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.400%
11) 1,1-Dichloroethene-d2	2.104	63	106094	3.561	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.200%
20) 2-Butanone-d5	3.899	46	147447	41.701	ug/L	-0.05
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.400%
24) Chloroform-d	4.346	84	102856	4.084	ug/L	0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.600%
26) 1,2-Dichloroethane-d4	5.030	65	55902	4.259	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
32) Benzene-d6	5.046	84	221595	3.886	ug/L	0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.800%
36) 1,2-Dichloropropane-d6	6.066	67	69930	3.801	ug/L	0.01
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.000%
41) Toluene-d8	7.313	98	182158	4.032	ug/L	0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.600%
43) trans-1,3-Dichloroprop...	7.625	79	17311	2.785	ug/L	0.02
Spiked Amount	5.000	Range	55 - 130	Recovery	=	55.600%
46) 2-Hexanone-d5	8.088	63	102861	38.339	ug/L	-0.01
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.680%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	46045	4.202	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.000%
66) 1,2-Dichlorobenzene-d4	11.619	152	55224	4.327	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.600%
Target Compounds						Qvalue
13) Acetone	2.185	43	29315	11.807	ug/L	88
31) Carbon tetrachloride	4.831	117	6103	0.318	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028570.D
Acq On : 15 Oct 2022 00:00
Operator : SY/MD
Sample : N5060-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1BC3

Quant Time: Oct 15 03:02:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 15 02:57:21 2022
Response via : Initial Calibration

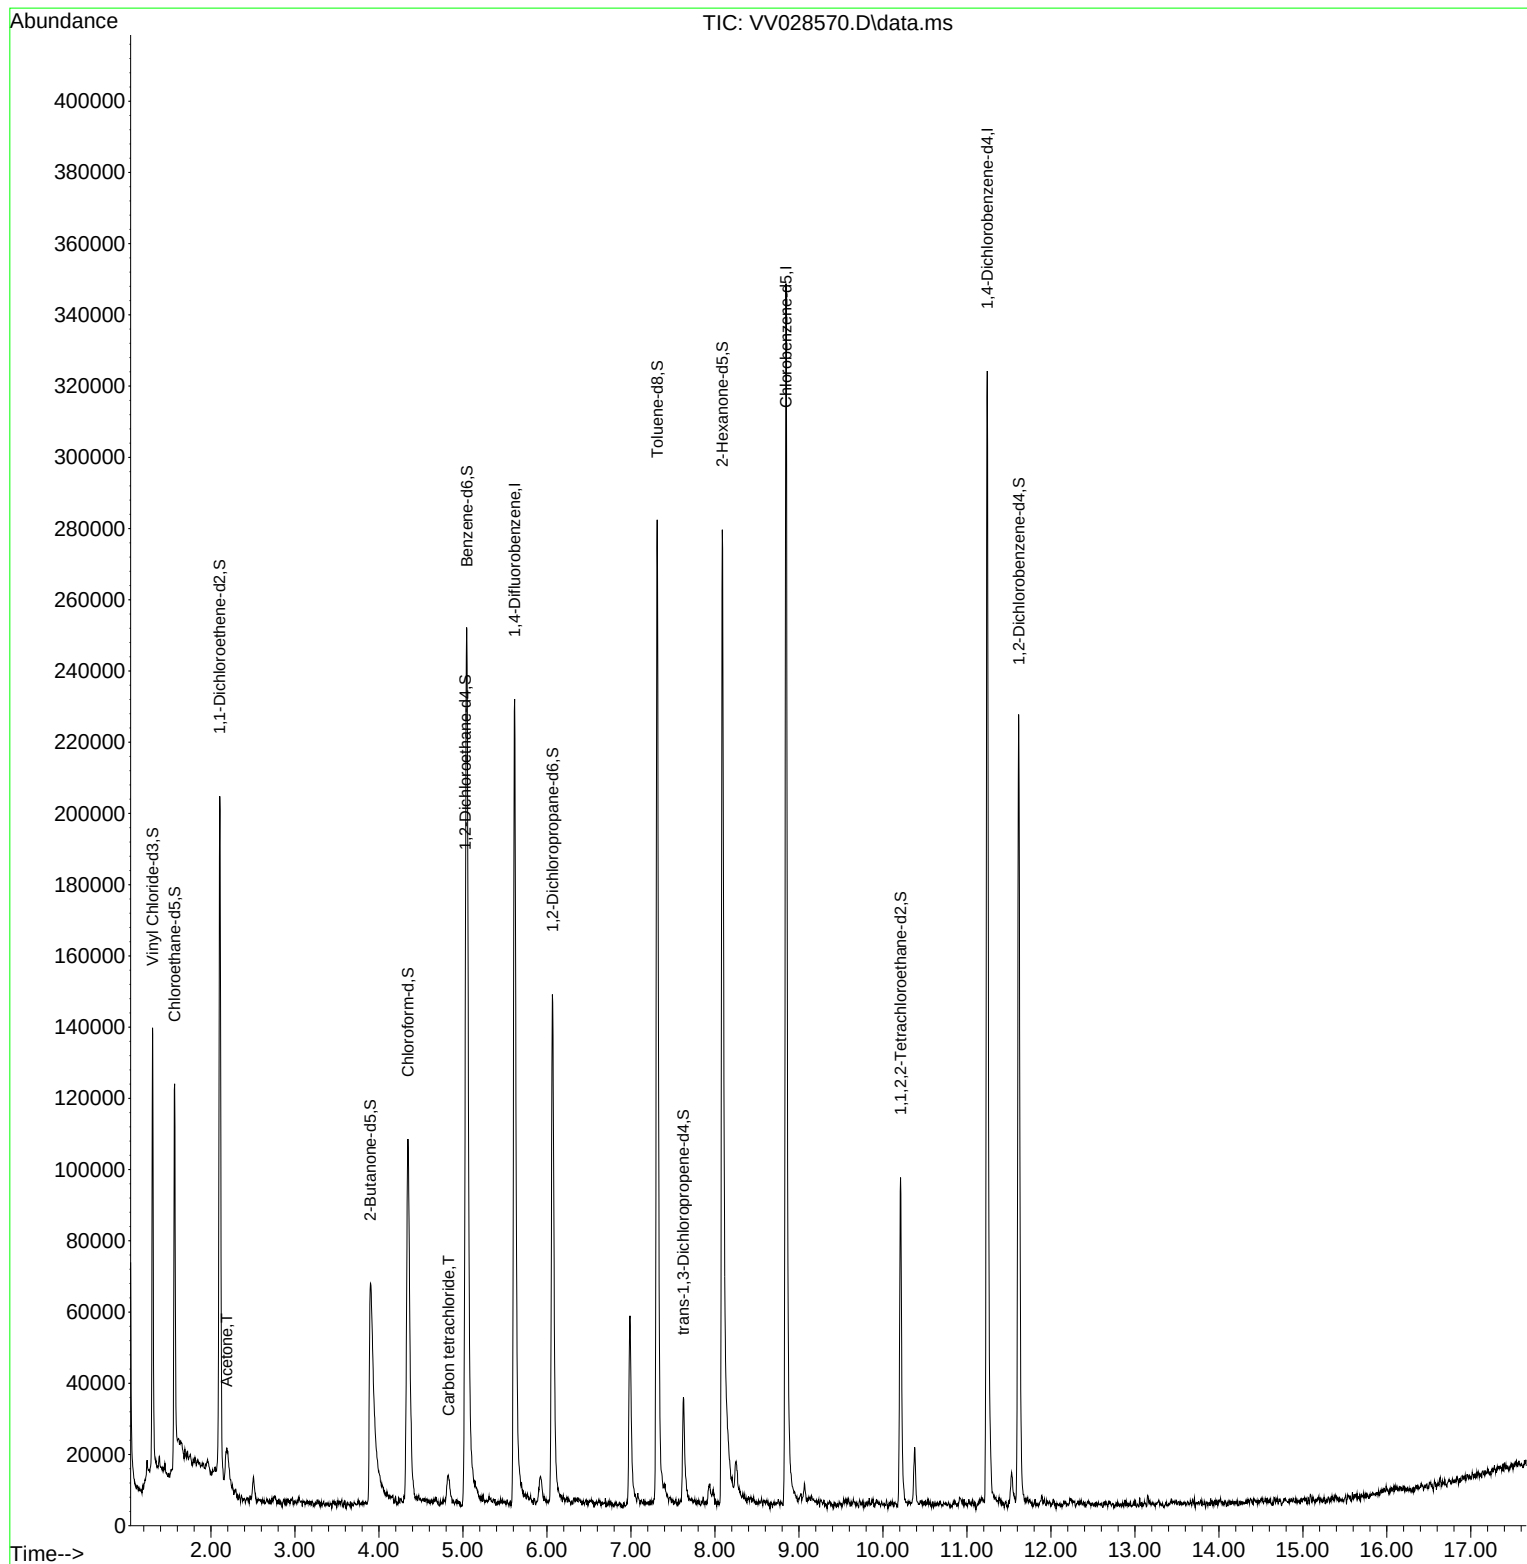

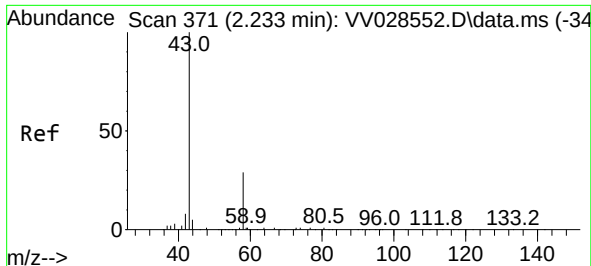

#13

Acetone

Concen: 11.807 ug/L

RT: 2.185 min Scan# 31

Delta R.T. -0.048 min

Lab File: VV028570.D

Acq: 15 Oct 2022 00:00

Instrument :

MSVOA_V

ClientSampleId :





C1BC3

Tgt Ion: 43 Resp: 29315

Ion Ratio Lower Upper

43 100

58 30.3 0.0 48.6

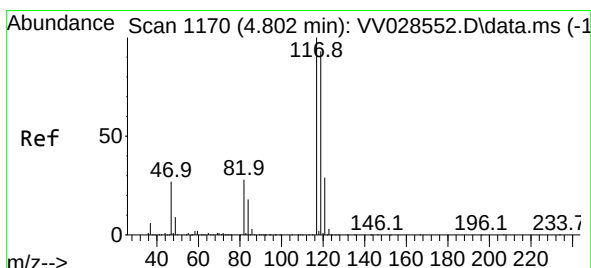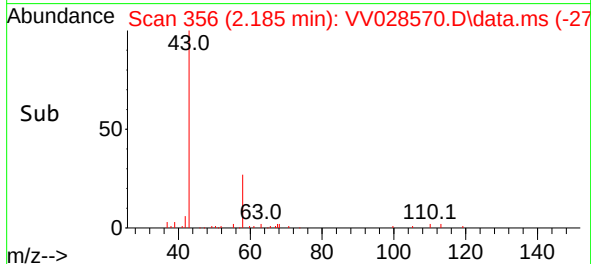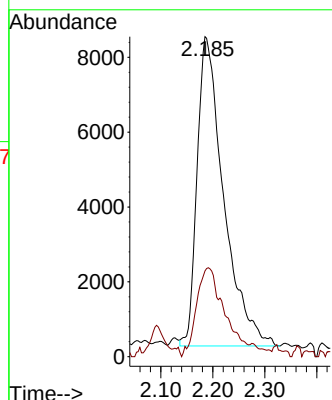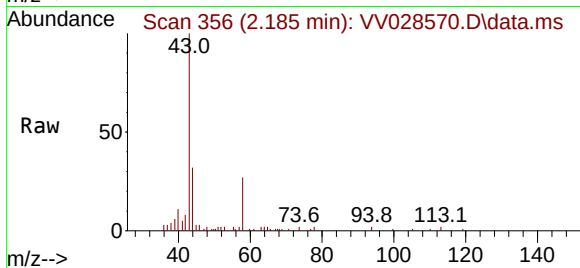

#31

Carbon tetrachloride

Concen: 0.318 ug/L

RT: 4.831 min Scan# 1179

Delta R.T. 0.029 min

Lab File: VV028570.D

Acq: 15 Oct 2022 00:00

Tgt Ion: 117 Resp: 6103

Ion Ratio Lower Upper

117 100

119 100.9 75.5 113.3

