

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028553.D
 Acq On : 14 Oct 2022 17:14
 Operator : SY/MD
 Sample : VV1014WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	50	60	61	rBV7	6630	9237	1.11%	0.138%
2	1.304	75	82	97	rVB	150822	149335	17.87%	2.229%
3	1.564	156	163	176	rBV	132161	149522	17.89%	2.231%
4	2.105	322	331	347	rVB	238154	348139	41.66%	5.195%
5	2.503	447	455	465	rBV2	15009	25489	3.05%	0.380%
6	3.941	889	902	903	rBV	29024	49460	5.92%	0.738%
7	4.342	1012	1027	1051	rVB	136361	351938	42.11%	5.252%
8	5.043	1228	1245	1276	rBV2	333791	835678	100.00%	12.471%
9	5.613	1411	1422	1448	rBV	268129	550912	65.92%	8.221%
10	6.066	1551	1563	1585	rBV	194940	405252	48.49%	6.048%
11	6.985	1838	1849	1867	rBV2	96018	182562	21.85%	2.724%
12	7.310	1938	1950	1971	rBV	378763	677124	81.03%	10.105%
13	7.622	2037	2047	2062	rBV2	51155	99062	11.85%	1.478%
14	8.092	2181	2193	2237	rBV	317705	805690	96.41%	12.023%
15	8.847	2416	2428	2448	rBV	397260	665353	79.62%	9.929%
16	10.210	2839	2852	2866	rBV	119624	201121	24.07%	3.001%
17	11.239	3162	3172	3195	rVV	391702	635146	76.00%	9.478%
18	11.616	3275	3289	3312	rBV	327189	544983	65.21%	8.133%
19	15.856	4598	4608	4610	rBV10	10322	15022	1.80%	0.224%




Sum of corrected areas: 6701025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028553.D
Acq On : 14 Oct 2022 17:14
Operator : SY/MD
Sample : VV1014WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

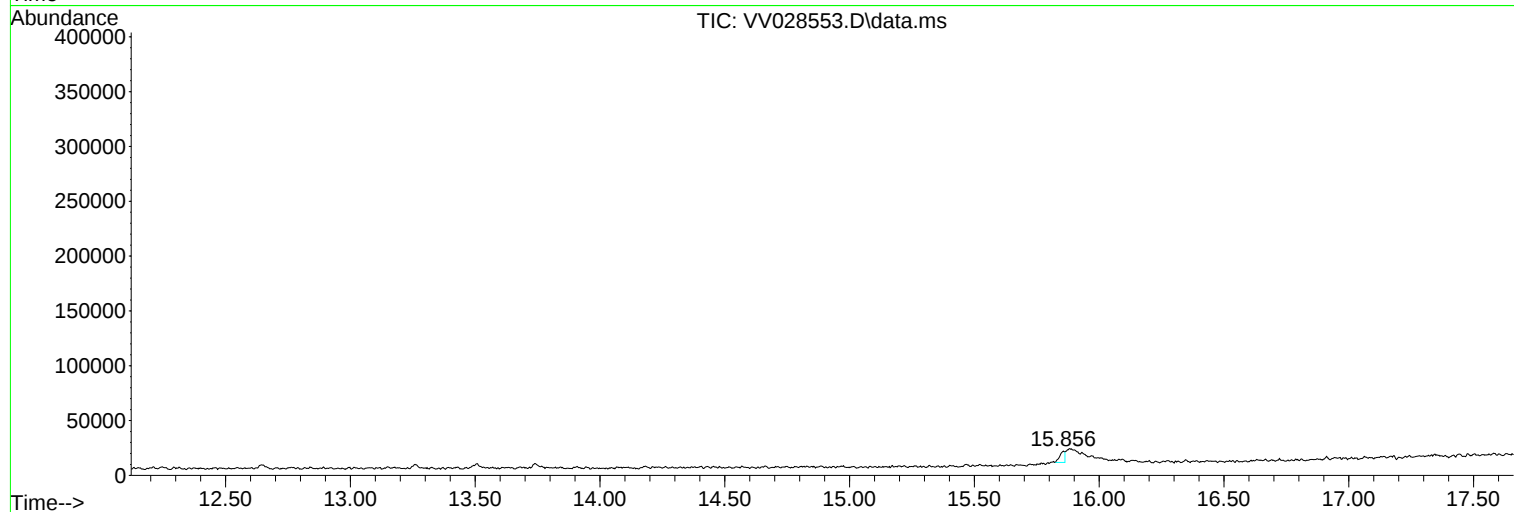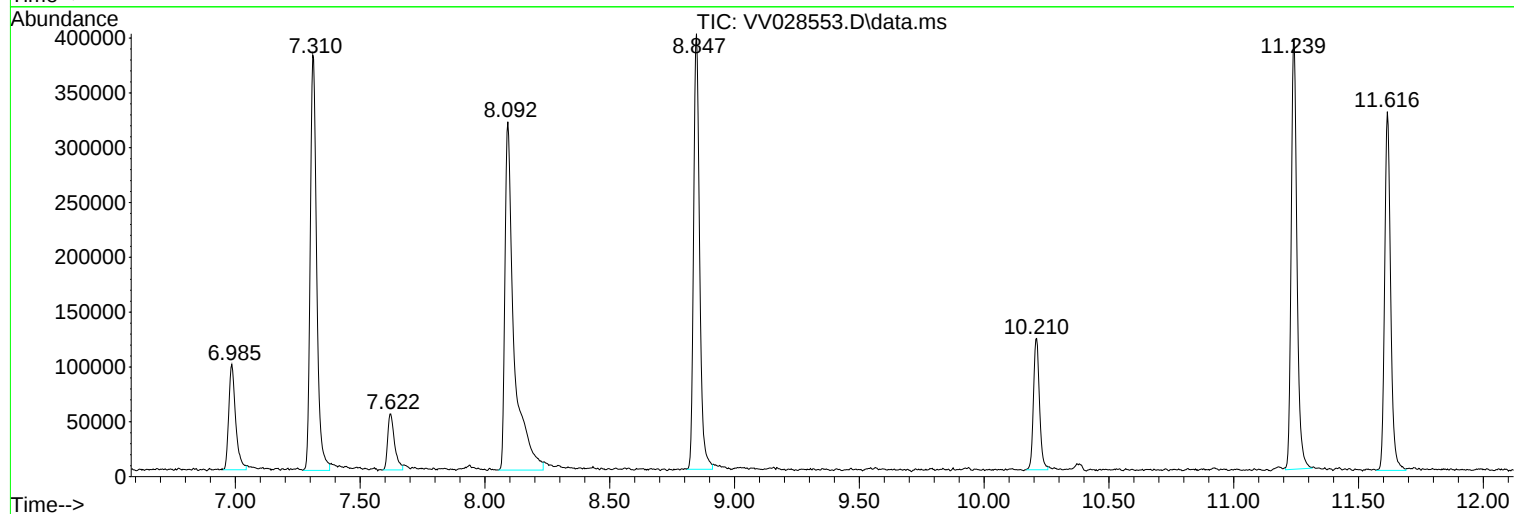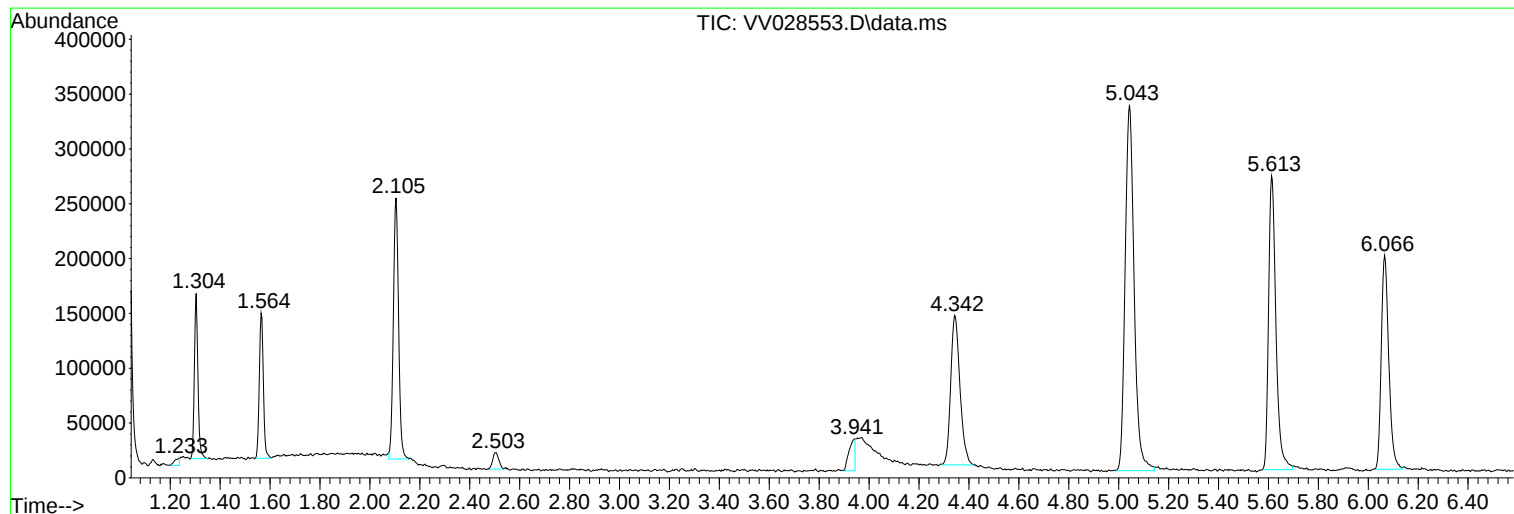

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028553.D
Acq On : 14 Oct 2022 17:14
Operator : SY/MD
Sample : VV1014WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028553.D
Acq On : 14 Oct 2022 17:14
Operator : SY/MD
Sample : VV1014WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc