

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028560.D
 Acq On : 14 Oct 2022 20:01
 Operator : SY/MD
 Sample : N5103-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	50	60	61	rBV2	7528	9467	1.45%	0.171%
2	1.304	75	82	98	rVB	148644	146424	22.37%	2.645%
3	1.564	156	163	173	rBV	121800	131672	20.11%	2.379%
4	2.104	321	331	346	rVB	222272	326328	49.85%	5.895%
5	2.503	448	455	461	rBV8	4384	6704	1.02%	0.121%
6	3.911	880	893	912	rBV2	33743	117659	17.97%	2.126%
7	4.346	1013	1028	1053	rVB	104956	268131	40.96%	4.844%
8	5.043	1230	1245	1269	rBV3	263306	654661	100.00%	11.826%
9	5.612	1411	1422	1446	rBV	242594	510180	77.93%	9.216%
10	6.066	1550	1563	1582	rBV	147459	312665	47.76%	5.648%
11	6.985	1837	1849	1868	rBV2	56373	112653	17.21%	2.035%
12	7.313	1940	1951	1970	rBV	303374	544010	83.10%	9.827%
13	7.622	2037	2047	2060	rBV3	31718	64886	9.91%	1.172%
14	7.931	2135	2143	2152	rBV2	7594	14015	2.14%	0.253%
15	8.091	2182	2193	2227	rBV	198832	536736	81.99%	9.696%
16	8.847	2417	2428	2455	rBV	362273	610831	93.30%	11.035%
17	10.210	2837	2852	2872	rBV	86136	156191	23.86%	2.822%
18	10.377	2894	2904	2916	rVB2	19752	33165	5.07%	0.599%
19	11.242	3161	3173	3192	rBV	349679	575830	87.96%	10.402%
20	11.615	3277	3289	3310	rBV	240032	403383	61.62%	7.287%




Sum of corrected areas: 5535591

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028560.D
Acq On : 14 Oct 2022 20:01
Operator : SY/MD
Sample : N5103-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

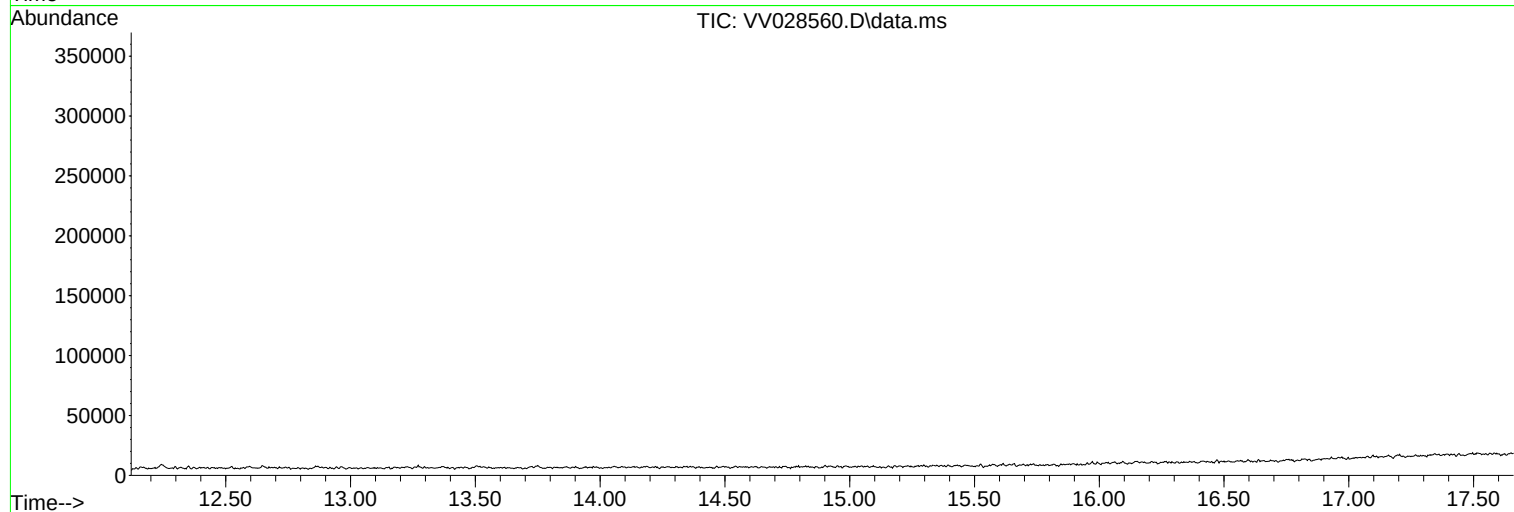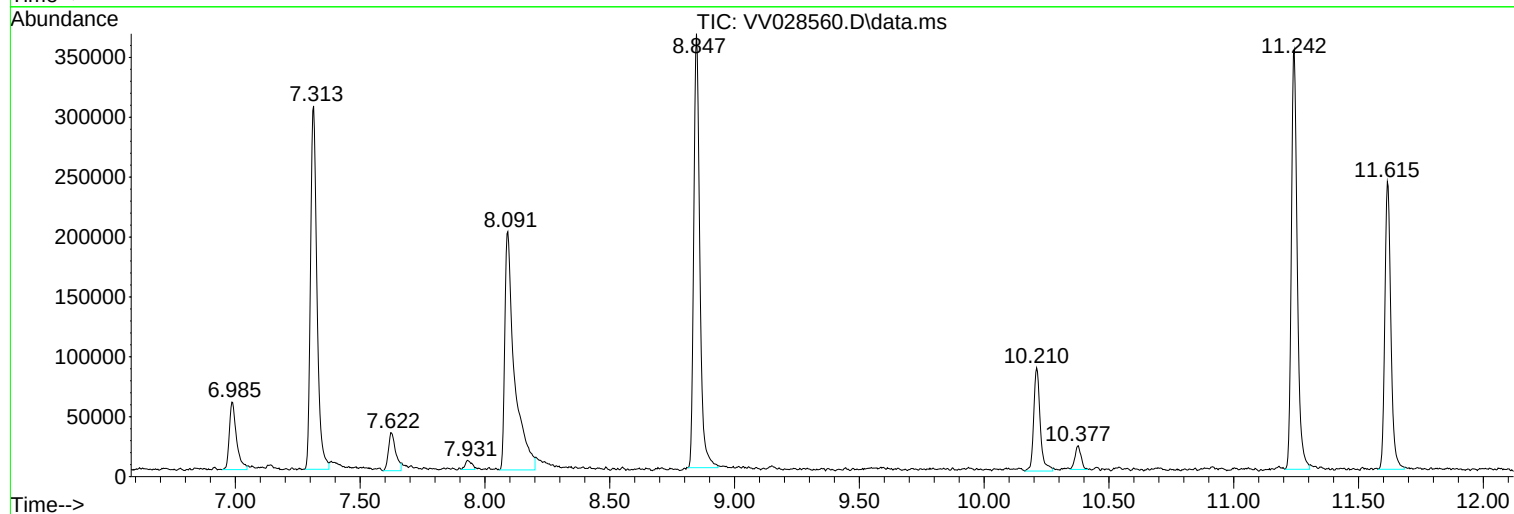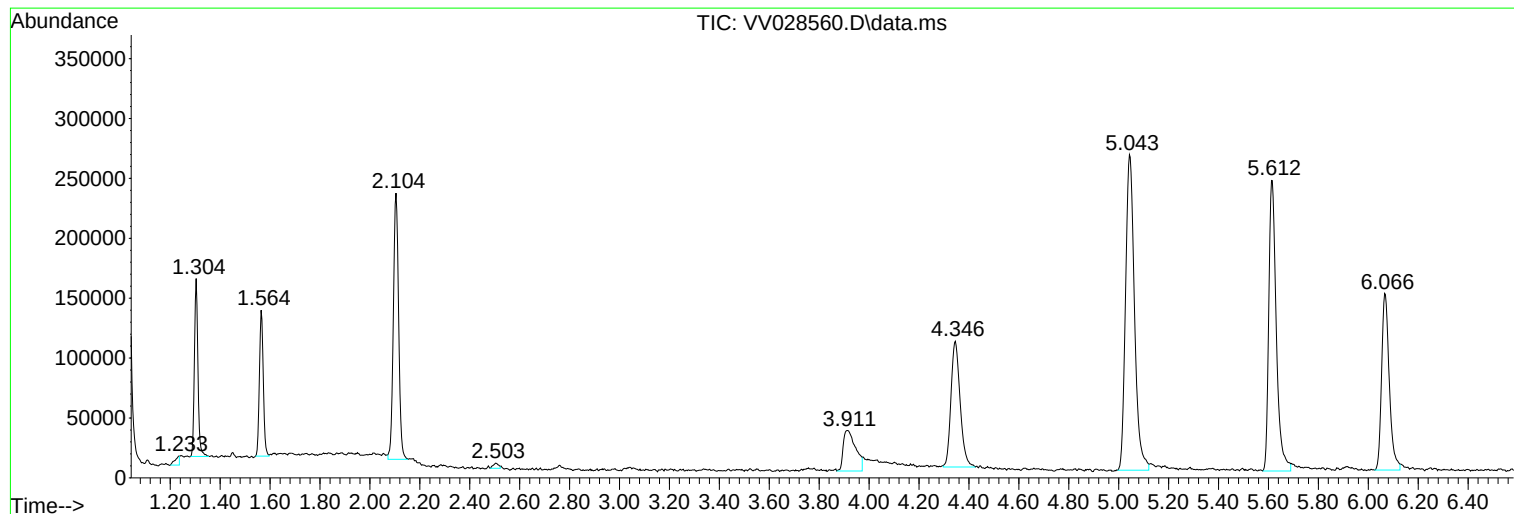

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028560.D
Acq On : 14 Oct 2022 20:01
Operator : SY/MD
Sample : N5103-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028560.D
Acq On : 14 Oct 2022 20:01
Operator : SY/MD
Sample : N5103-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc