

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028564.D
 Acq On : 14 Oct 2022 21:37
 Operator : SY/MD
 Sample : N5103-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BX3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rBV	128840	134804	20.95%	2.462%
2	1.568	155	164	173	rBV	108098	126510	19.66%	2.311%
3	2.105	322	331	344	rVB	199730	293392	45.59%	5.359%
4	2.503	445	455	468	rVB2	9217	17172	2.67%	0.314%
5	3.902	875	890	919	rBV2	59034	217388	33.78%	3.970%
6	4.346	1014	1028	1051	rVB2	102347	262425	40.78%	4.793%
7	5.043	1228	1245	1271	rBV3	252371	643578	100.00%	11.754%
8	5.616	1411	1423	1447	rBV	236713	492543	76.53%	8.996%
9	6.066	1550	1563	1585	rBV	149156	317490	49.33%	5.799%
10	6.989	1840	1850	1865	rBV	55076	108292	16.83%	1.978%
11	7.313	1936	1951	1972	rBV	284827	511231	79.44%	9.337%
12	7.625	2039	2048	2060	rBV3	28986	56116	8.72%	1.025%
13	7.934	2135	2144	2152	rBV4	5638	10986	1.71%	0.201%
14	8.088	2182	2192	2227	rBV	270275	589429	91.59%	10.765%
15	8.847	2415	2428	2448	rBV	347925	593305	92.19%	10.836%
16	10.210	2839	2852	2865	rBV	91766	155449	24.15%	2.839%
17	10.378	2895	2904	2915	rVB3	13220	23790	3.70%	0.435%
18	11.243	3162	3173	3196	rBV	319969	539672	83.85%	9.857%
19	11.619	3278	3290	3306	rBV	226100	381652	59.30%	6.971%




Sum of corrected areas: 5475224

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028564.D
Acq On : 14 Oct 2022 21:37
Operator : SY/MD
Sample : N5103-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

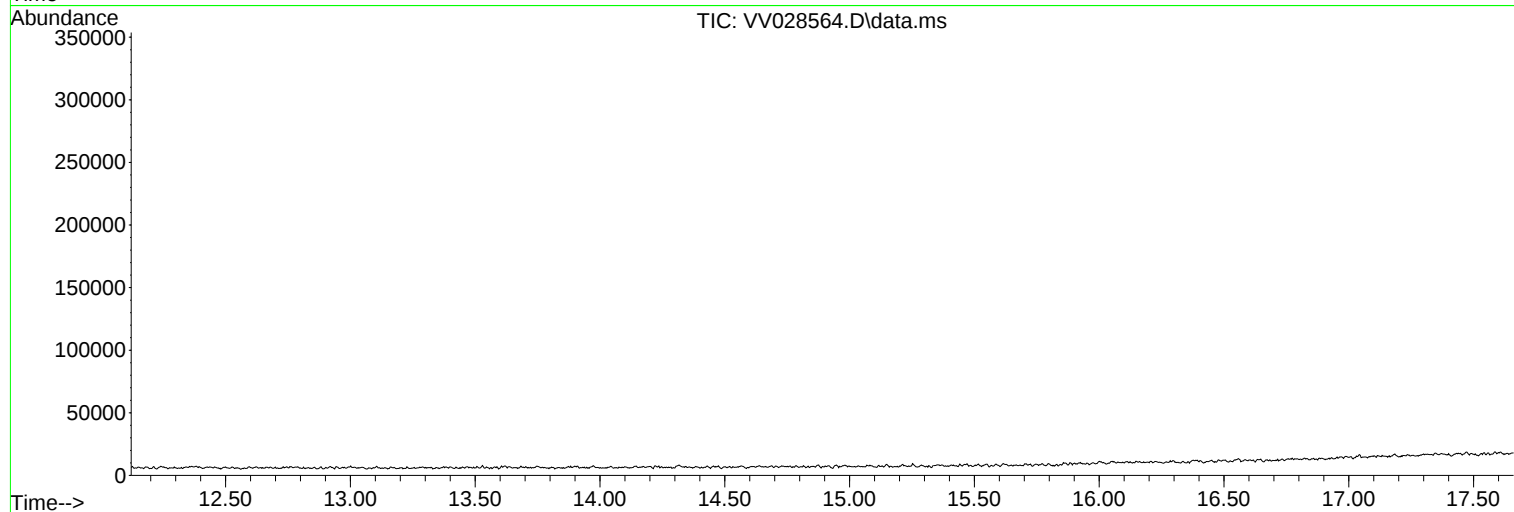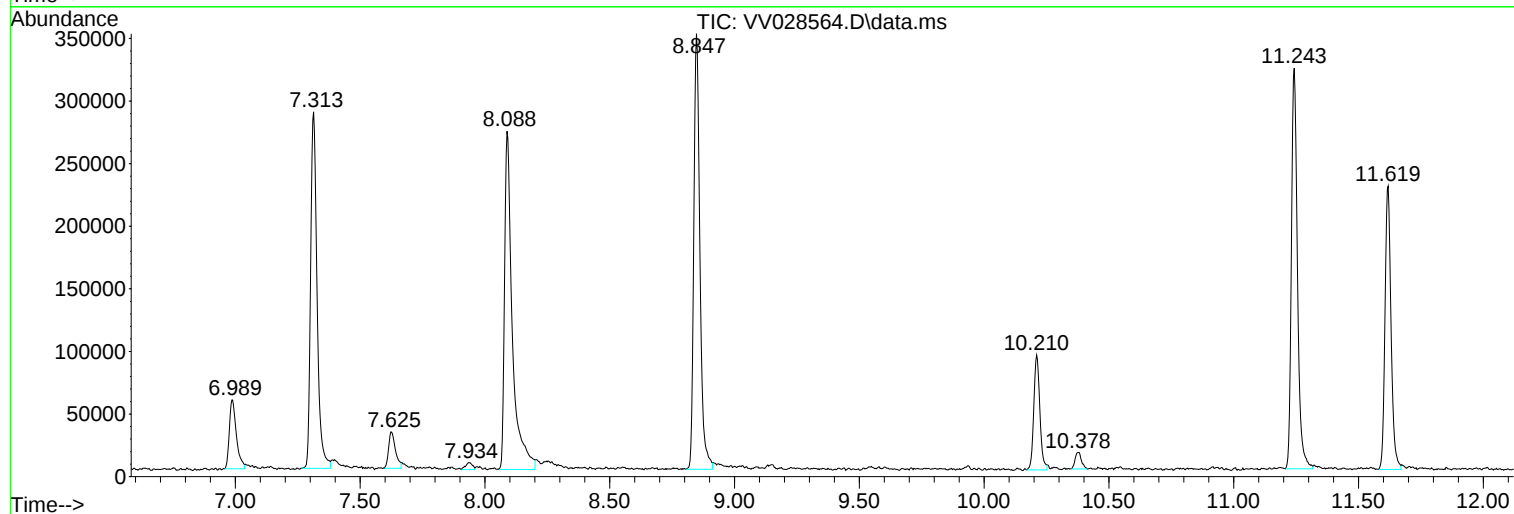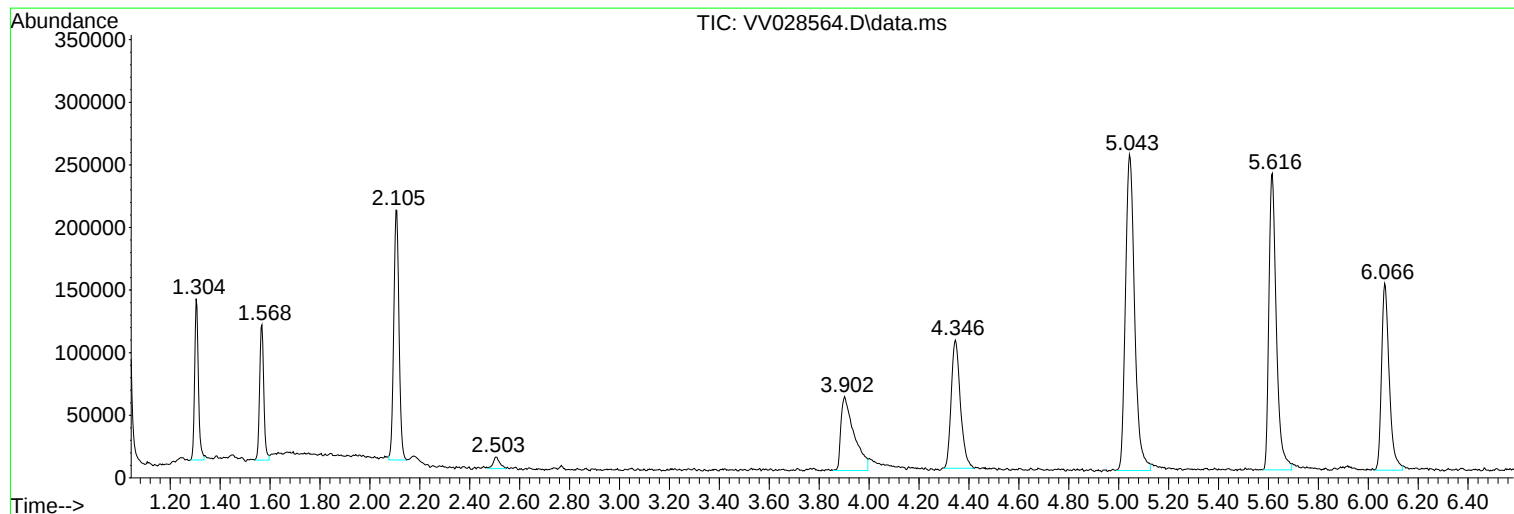

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028564.D
Acq On : 14 Oct 2022 21:37
Operator : SY/MD
Sample : N5103-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
Data File : VV028564.D
Acq On : 14 Oct 2022 21:37
Operator : SY/MD
Sample : N5103-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc