
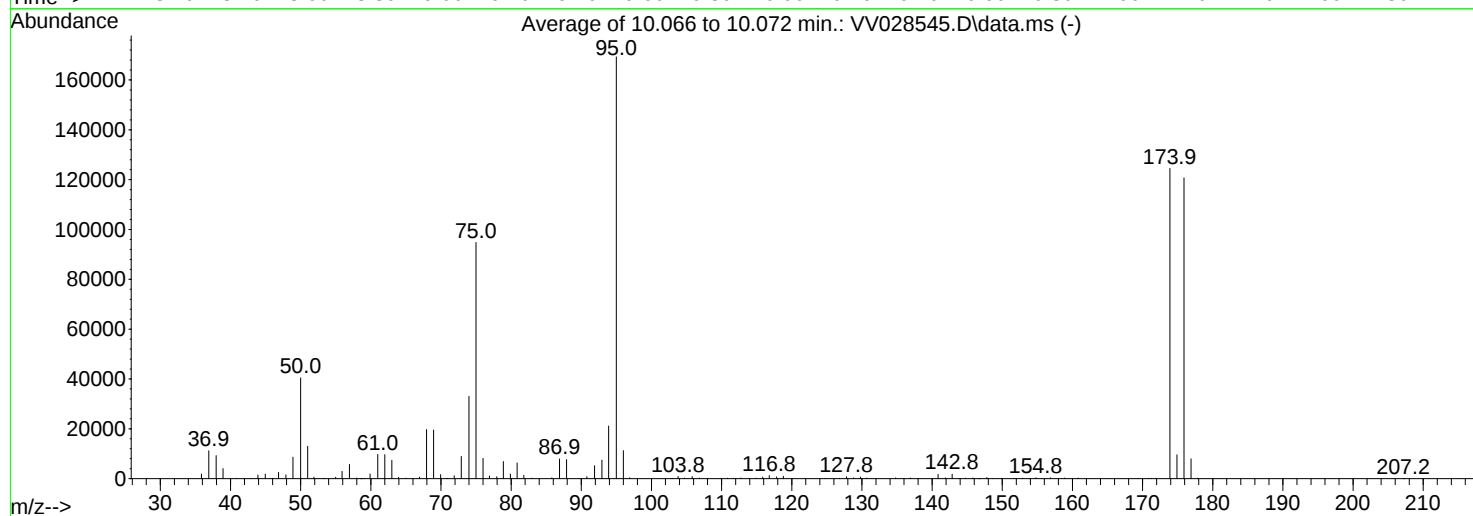


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101422\
 Data File : VV028545.D
 Acq On : 14 Oct 2022 11:11
 Operator : SY/MD
 Sample : BFB384
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB384

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Oct 18 01:19:01 2022

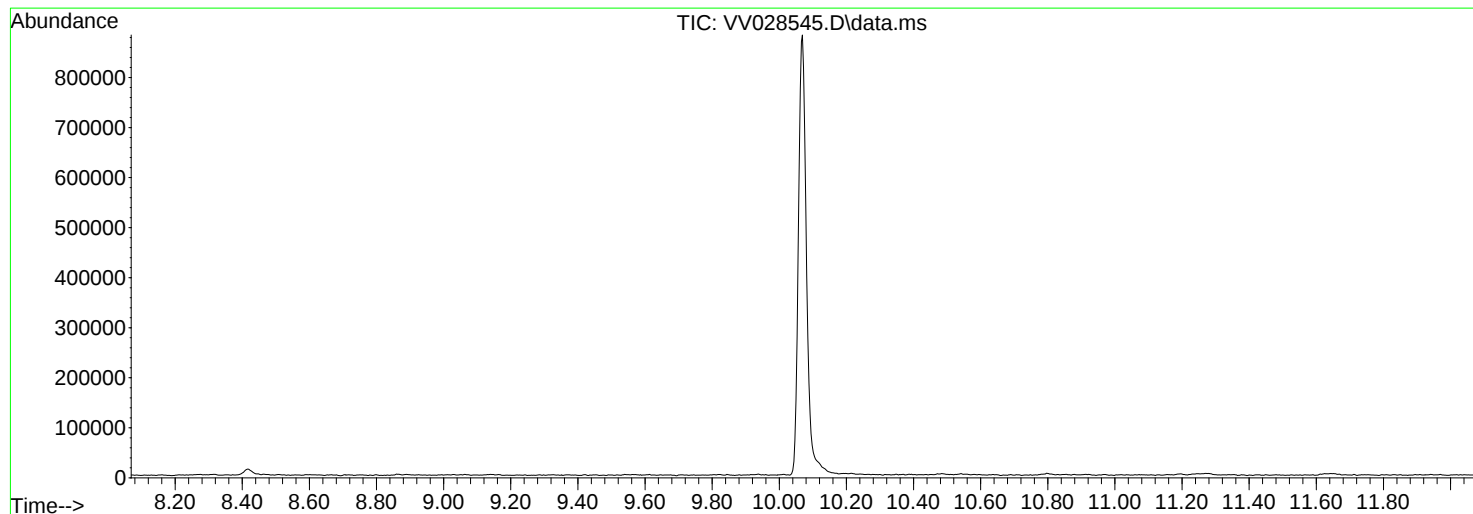

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	40477	PASS
75	95	30	80	56.0	94795	PASS
95	95	100	100	100.0	169280	PASS
96	95	5	9	6.7	11267	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.6	124509	PASS
175	174	5	9	7.7	9578	PASS
176	174	95	105	97.0	120741	PASS
177	176	5	10	6.6	7939	PASS

m/z	Abundance
35.70	135.0
36.20	114.0
36.80	115.0
37.30	138.0
37.80	151.0
38.00	151.0
39.00	152.0
39.80	1188.0
40.80	121.0
41.20	129.0
42.00	159.0
43.00	226.0
43.90	1110.0
44.70	140.0
45.50	137.0
46.10	131.0
46.80	104.0
48.90	139.0
49.70	139.0
51.20	159.0
52.70	135.0
55.90	243.0
56.90	136.0
57.40	111.0
58.10	114.0
61.10	119.0
63.80	107.0
67.20	133.0
70.00	137.0
73.70	105.0
76.90	118.0
80.80	107.0
126.40	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

m/z	Abundance
35.90	1990.0
37.00	11503.0
38.00	10018.0
39.00	4388.0
39.90	1069.0
41.00	228.0
41.90	110.0
42.90	303.0
43.90	2767.0
45.00	1960.0
45.90	250.0
46.90	2767.0
47.90	1458.0
49.00	9210.0
50.00	41704.0
51.00	13621.0
51.90	606.0
53.20	235.0
55.00	596.0
55.90	3199.0
57.00	5911.0
58.00	369.0
58.60	118.0
59.10	146.0
59.90	1959.0
61.00	10202.0
62.00	9534.0
63.00	7615.0
64.00	673.0
64.90	203.0
67.00	755.0
68.00	20008.0
68.90	19992.0
69.90	1726.0
71.00	182.0
71.90	1278.0
72.90	9321.0
74.00	34016.0
75.00	96568.0
76.00	8501.0
76.90	1328.0
77.90	731.0
78.90	6756.0
79.90	1877.0
80.90	6412.0
81.80	1330.0
82.90	192.0
85.70	324.0
86.90	8132.0
87.90	7833.0
90.80	723.0
91.90	5341.0
92.90	7611.0
93.90	21120.0
95.00	173312.0
96.00	11714.0
96.90	379.0
102.80	109.0
103.80	919.0
104.70	248.0
105.80	896.0
106.90	203.0
109.90	176.0
110.90	191.0
111.70	171.0
112.70	292.0
114.90	216.0
115.90	640.0
116.80	1344.0
117.80	682.0
118.80	927.0
124.80	105.0
126.80	104.0
127.80	758.0
128.80	288.0
129.80	682.0
130.70	235.0
134.80	367.0
136.90	284.0
139.90	147.0
140.90	1823.0
141.90	344.0
142.80	1815.0
143.90	108.0
144.90	208.0
145.70	292.0
146.70	104.0
147.80	493.0
148.60	142.0
149.80	142.0
151.90	123.0
152.90	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

153.80	156.0
154.80	365.0
156.80	300.0
158.90	291.0
160.80	248.0
169.30	119.0
170.90	149.0
171.90	401.0
173.90	123992.0
174.90	10029.0
175.90	119592.0
176.90	8030.0
177.80	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

m/z	Abundance
35.90	2038.0
36.90	11580.0
38.00	9794.0
38.90	4359.0
39.80	1047.0
40.90	249.0
41.90	166.0
42.90	303.0
43.90	2693.0
44.90	1866.0
45.90	258.0
46.90	2680.0
47.90	1657.0
49.00	8941.0
50.00	41760.0
51.00	13644.0
51.90	701.0
53.20	200.0
55.00	643.0
55.90	3260.0
57.00	6044.0
58.00	353.0
59.10	100.0
59.90	1908.0
61.00	10065.0
62.00	9900.0
63.00	7529.0
64.00	654.0
65.00	215.0
67.00	706.0
67.90	20312.0
68.90	19992.0
69.90	1816.0
70.90	145.0
71.90	1160.0
72.90	9194.0
74.00	34000.0
75.00	97792.0
76.00	8406.0
76.90	1276.0
78.00	791.0
78.90	7086.0
79.90	1935.0
80.90	6547.0
81.80	1372.0
83.00	177.0
85.80	330.0
86.90	8125.0
87.90	7905.0
89.70	106.0
90.80	839.0
91.90	5458.0
92.90	7637.0
93.90	21688.0
95.00	174272.0
96.00	11597.0
96.90	360.0
102.80	112.0
103.80	936.0
104.70	293.0
105.80	904.0
106.80	240.0
107.90	101.0
109.90	136.0
110.90	168.0
111.70	162.0
112.80	295.0
114.90	224.0
115.80	659.0
116.80	1255.0
117.80	695.0
118.80	1000.0
124.70	114.0
126.80	109.0
127.80	806.0
128.80	337.0
129.80	659.0
130.70	261.0
134.80	349.0
136.90	271.0
140.80	1809.0
141.90	312.0
142.90	1835.0
143.70	111.0
144.70	186.0
145.80	277.0
147.80	520.0
148.70	116.0
149.90	139.0
151.60	102.0
152.00	102.0
152.90	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

153.80	135.0
154.80	365.0
156.90	347.0
158.90	234.0
160.80	259.0
169.40	122.0
170.90	165.0
171.30	172.0
173.90	128512.0
174.90	9832.0
175.90	124808.0
176.90	8248.0
177.80	200.0
207.20	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

m/z	Abundance
35.90	1946.0
36.90	10761.0
38.00	8930.0
38.90	3896.0
39.90	963.0
40.90	219.0
41.90	217.0
42.90	305.0
43.90	2354.0
44.90	1823.0
45.90	231.0
46.90	2313.0
47.90	1570.0
48.90	8129.0
50.00	37968.0
51.00	12130.0
51.90	707.0
52.90	163.0
53.40	162.0
55.00	607.0
55.90	3064.0
57.00	5605.0
58.00	345.0
59.90	1779.0
61.00	9120.0
62.00	9446.0
63.00	6819.0
64.00	571.0
65.10	260.0
66.90	549.0
67.90	18768.0
69.00	18512.0
70.00	1764.0
70.80	124.0
71.90	1032.0
72.90	8329.0
74.00	30976.0
75.00	90024.0
76.00	7569.0
76.90	1091.0
78.00	759.0
78.90	6717.0
79.90	1810.0
80.90	6160.0
81.80	1276.0
82.90	191.0
85.90	373.0
86.90	7414.0
87.90	7263.0
89.70	117.0
90.80	871.0
91.90	4882.0
93.00	7186.0
93.90	20664.0
95.00	160256.0
96.00	10490.0
96.90	340.0
103.00	123.0
103.80	852.0
104.70	317.0
105.80	807.0
106.80	300.0
109.90	103.0
110.80	144.0
111.70	148.0
112.80	282.0
114.90	224.0
115.80	599.0
116.80	1078.0
117.90	673.0
118.80	902.0
124.80	105.0
126.80	110.0
127.80	780.0
128.80	342.0
129.80	575.0
130.70	268.0
134.80	314.0
136.90	291.0
139.90	115.0
140.80	1631.0
141.90	253.0
142.90	1671.0
143.80	113.0
144.70	195.0
145.90	236.0
147.80	441.0
149.90	151.0
151.60	103.0
152.90	217.0
154.80	352.0
156.90	336.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

158.80	173.0
160.80	224.0
169.40	108.0
170.90	154.0
171.30	163.0
173.90	121024.0
174.90	8872.0
175.90	117824.0
176.90	7540.0
177.90	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384