

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037848.D
 Acq On : 14 Oct 2024 11:48
 Operator : SY/MD
 Sample : P4349-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 15 02:21:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 15 02:19:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	544469	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	546503	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	249173	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	164630	34.445	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	68.880%
7) Chloroethane-d5	1.532	69	157952	42.575	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.160%
11) 1,1-Dichloroethene-d2	2.059	65	81576	40.852	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.700%
21) 2-Butanone-d5	3.796	46	189832	111.509	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.510%
24) Chloroform-d	4.243	84	419192	49.297	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.600%
26) 1,2-Dichloroethane-d4	4.937	65	260272	52.292	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.580%
32) Benzene-d6	4.953	84	792963	46.369	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.740%
36) 1,2-Dichloropropane-d6	5.985	67	268074	49.228	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.460%
41) Toluene-d8	7.236	98	676008	43.594	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.180%
43) trans-1,3-Dichloroprop...	7.548	79	109607	43.329	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.660%
47) 2-Hexanone-d5	8.024	63	114394	99.484	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.480%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	326536	51.608	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.220%
66) 1,2-Dichlorobenzene-d4	11.554	152	274877	52.352	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.700%
Target Compounds						
61) 1,2,3-Trichloropropane	11.178	75	29175	8.228	ug/L	Qvalue # 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037848.D
Acq On : 14 Oct 2024 11:48
Operator : SY/MD
Sample : P4349-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 15 02:21:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 15 02:19:17 2024
Response via : Initial Calibration

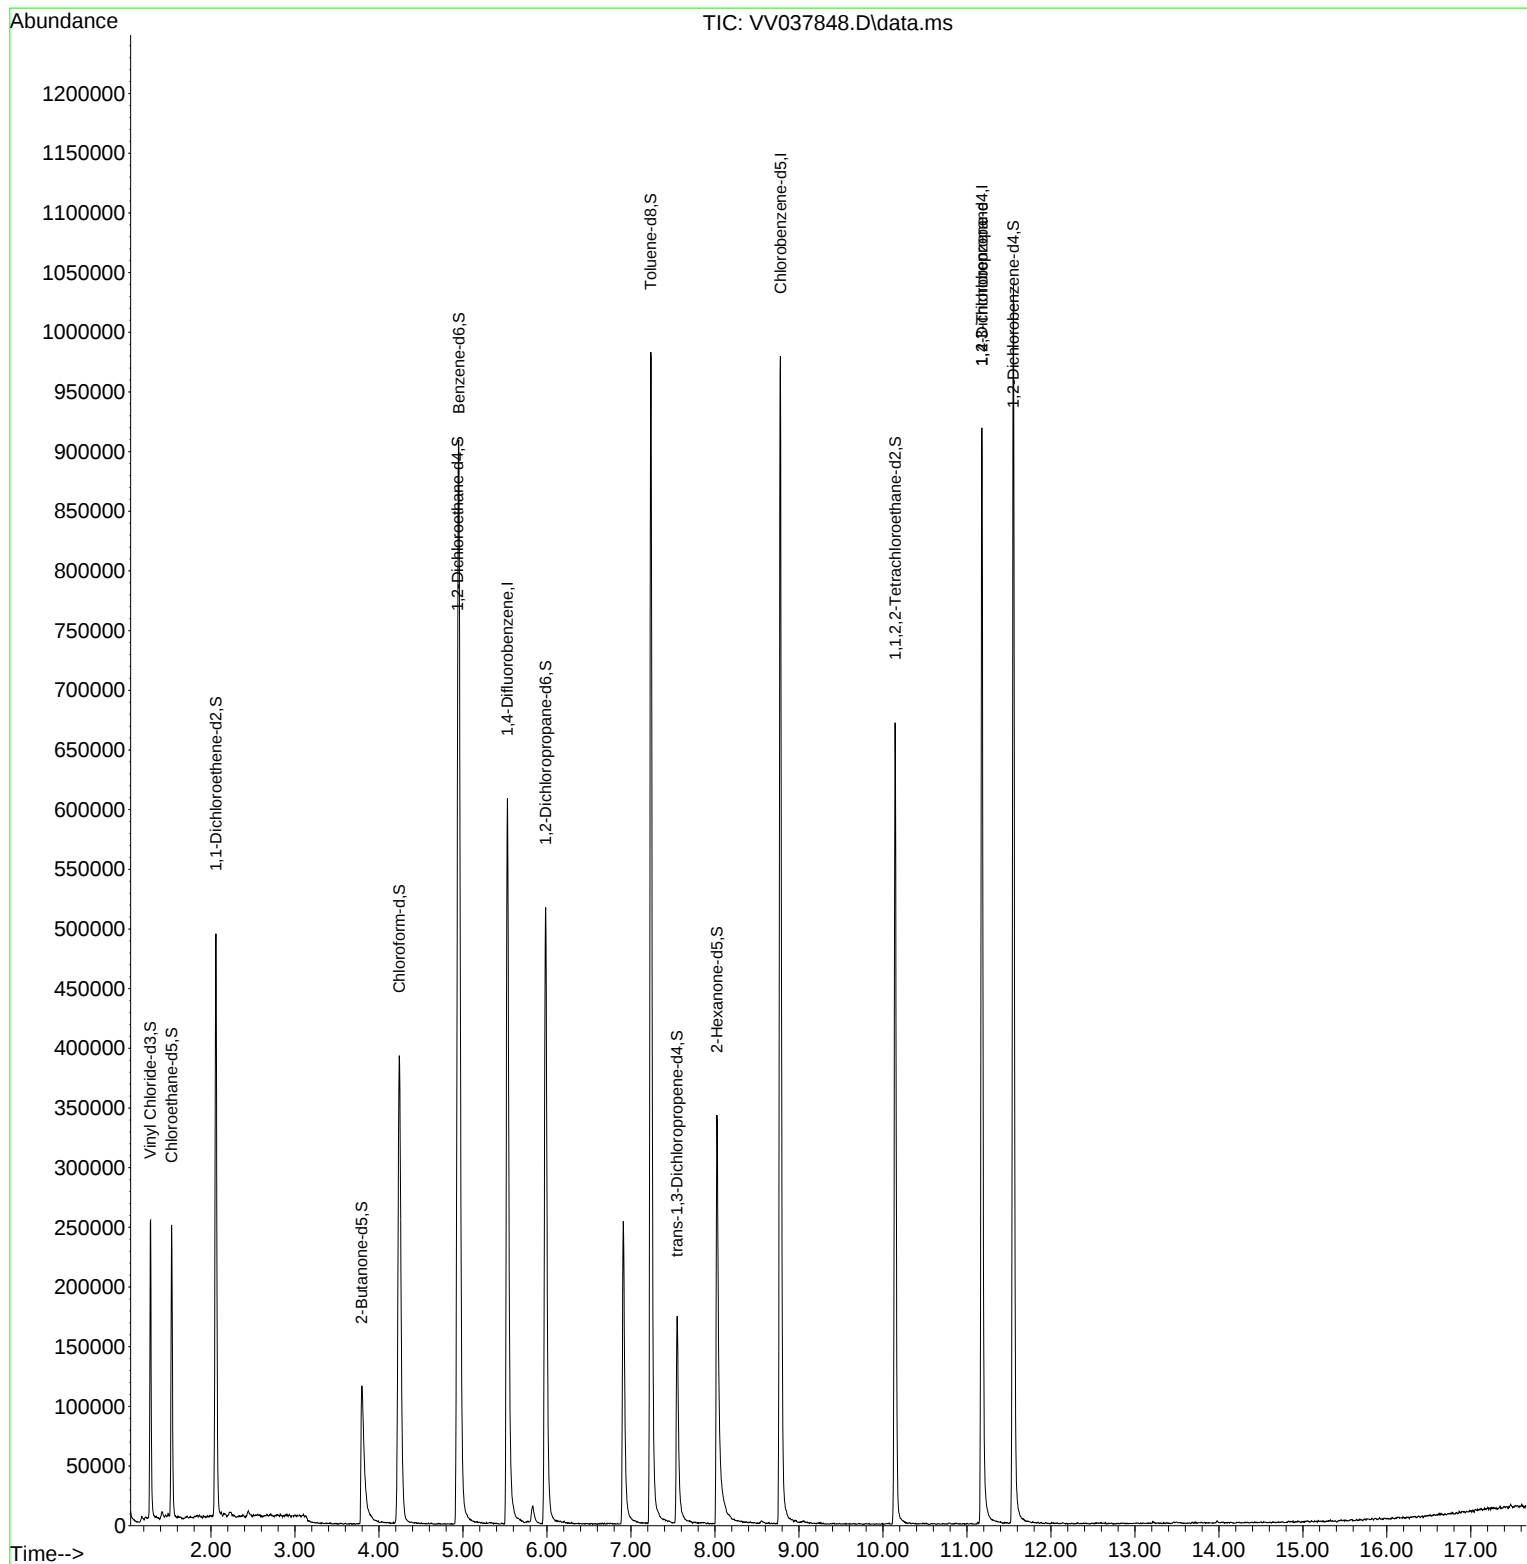

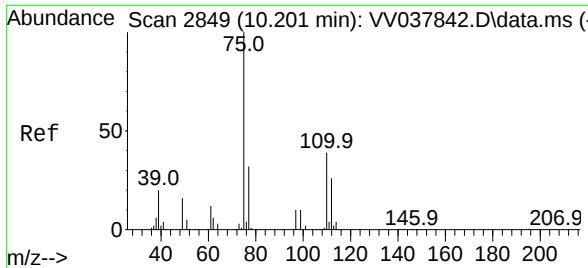

#61
 1,2,3-Trichloropropane
 Concen: 8.228 ug/L
 RT: 11.178 min Scan# 31
 Delta R.T. 0.977 min
 Lab File: VV037848.D
 Acq: 14 Oct 2024 11:48

Instrument :
 MSVOA_V
 ClientSampleId :

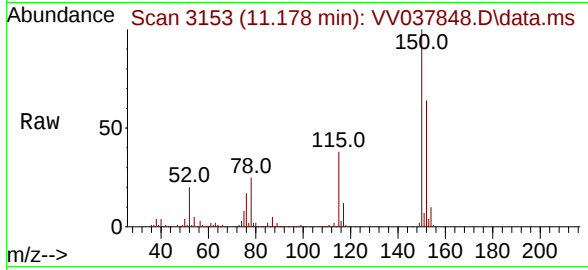

Tgt Ion: 75 Resp: 29175

Ion	Ratio	Lower	Upper
75	100		
77	31.6	25.4	38.0
110	2.8	31.7	47.5#

