

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037851.D
 Acq On : 14 Oct 2024 13:08
 Operator : SY/MD
 Sample : P4379-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 15 02:21:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 15 02:19:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	763492	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	740711	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	346184	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	196228	29.278	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	58.560%#
7) Chloroethane-d5	1.532	69	175516	33.738	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	67.480%#
11) 1,1-Dichloroethene-d2	2.057	65	95478	34.098	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.200%
21) 2-Butanone-d5	3.793	46	180774	75.726	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	75.730%
24) Chloroform-d	4.236	84	452752	37.969	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.940%
26) 1,2-Dichloroethane-d4	4.931	65	276974	39.684	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.360%
32) Benzene-d6	4.947	84	880177	37.974	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.940%
36) 1,2-Dichloropropane-d6	5.979	67	284522	38.550	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	77.100%
41) Toluene-d8	7.233	98	767415	36.513	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	73.020%#
43) trans-1,3-Dichloroprop...	7.548	79	116284	33.916	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.840%
47) 2-Hexanone-d5	8.021	63	111231	71.371	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	71.370%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	320747	37.401	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	74.800%
66) 1,2-Dichlorobenzene-d4	11.551	152	307501	42.153	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.300%
Target Compounds						
61) 1,2,3-Trichloropropane	11.178	75	41189	8.361	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037851.D
Acq On : 14 Oct 2024 13:08
Operator : SY/MD
Sample : P4379-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 15 02:21:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 15 02:19:17 2024
Response via : Initial Calibration

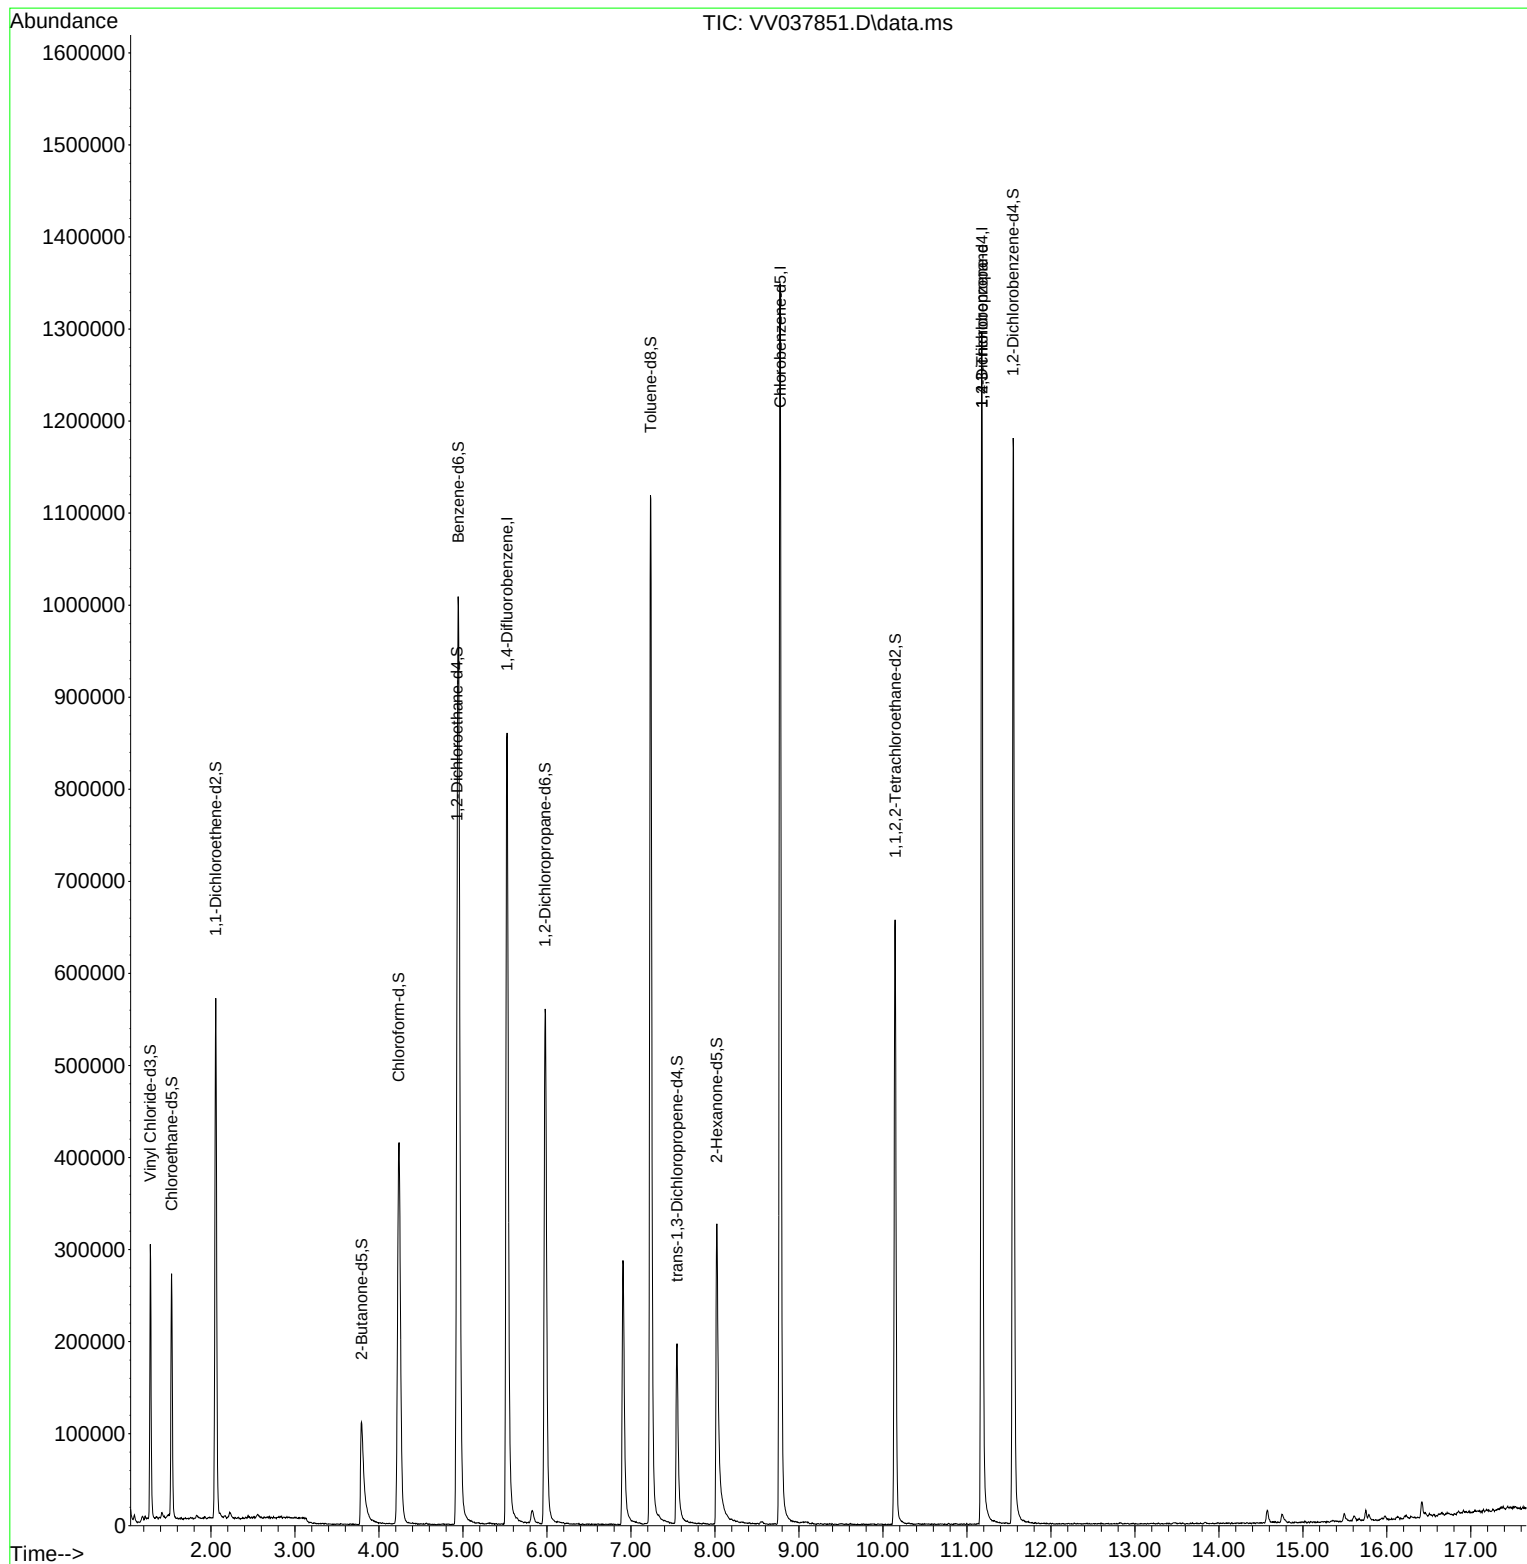

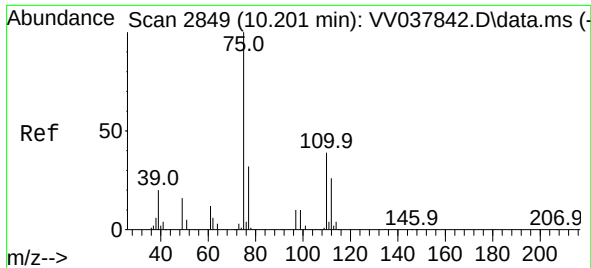

#61

1,2,3-Trichloropropane

Concen: 8.361 ug/L

RT: 11.178 min Scan# 31

Delta R.T. 0.978 min


Lab File: VV037851.D

Acq: 14 Oct 2024 13:08

Instrument :

MSVOA_V

ClientSampleId :

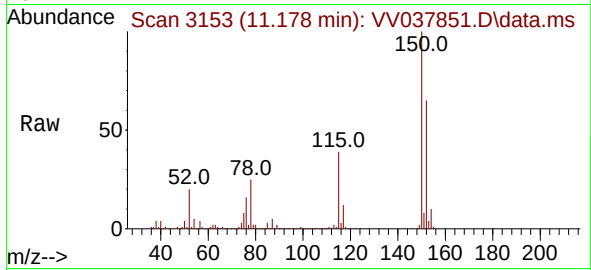

Tgt Ion: 75 Resp: 41189

Ion Ratio Lower Upper

75 100

77 33.6 25.4 38.0

110 3.0 31.7 47.5#

