

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037854.D
 Acq On : 14 Oct 2024 14:12
 Operator : SY/MD
 Sample : P4378-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 15 02:22:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 15 02:19:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	618003	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	612155	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	274950	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	167537	30.882	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	61.760%
7) Chloroethane-d5	1.532	69	155131	36.839	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	73.680%
11) 1,1-Dichloroethene-d2	2.060	65	81014	35.743	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.480%
21) 2-Butanone-d5	3.799	46	160265	82.940	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.940%
24) Chloroform-d	4.243	84	406705	42.137	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.280%
26) 1,2-Dichloroethane-d4	4.937	65	249270	44.123	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.240%
32) Benzene-d6	4.953	84	790025	41.243	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.480%
36) 1,2-Dichloropropane-d6	5.982	67	256625	42.072	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.140%
41) Toluene-d8	7.236	98	687376	39.573	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.140%#
43) trans-1,3-Dichloroprop...	7.551	79	107205	37.834	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.660%
47) 2-Hexanone-d5	8.024	63	100912	78.347	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.350%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	293709	41.441	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.880%
66) 1,2-Dichlorobenzene-d4	11.554	152	276934	47.799	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	11.178	75	31183	7.970	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037854.D
Acq On : 14 Oct 2024 14:12
Operator : SY/MD
Sample : P4378-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 15 02:22:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 15 02:19:17 2024
Response via : Initial Calibration

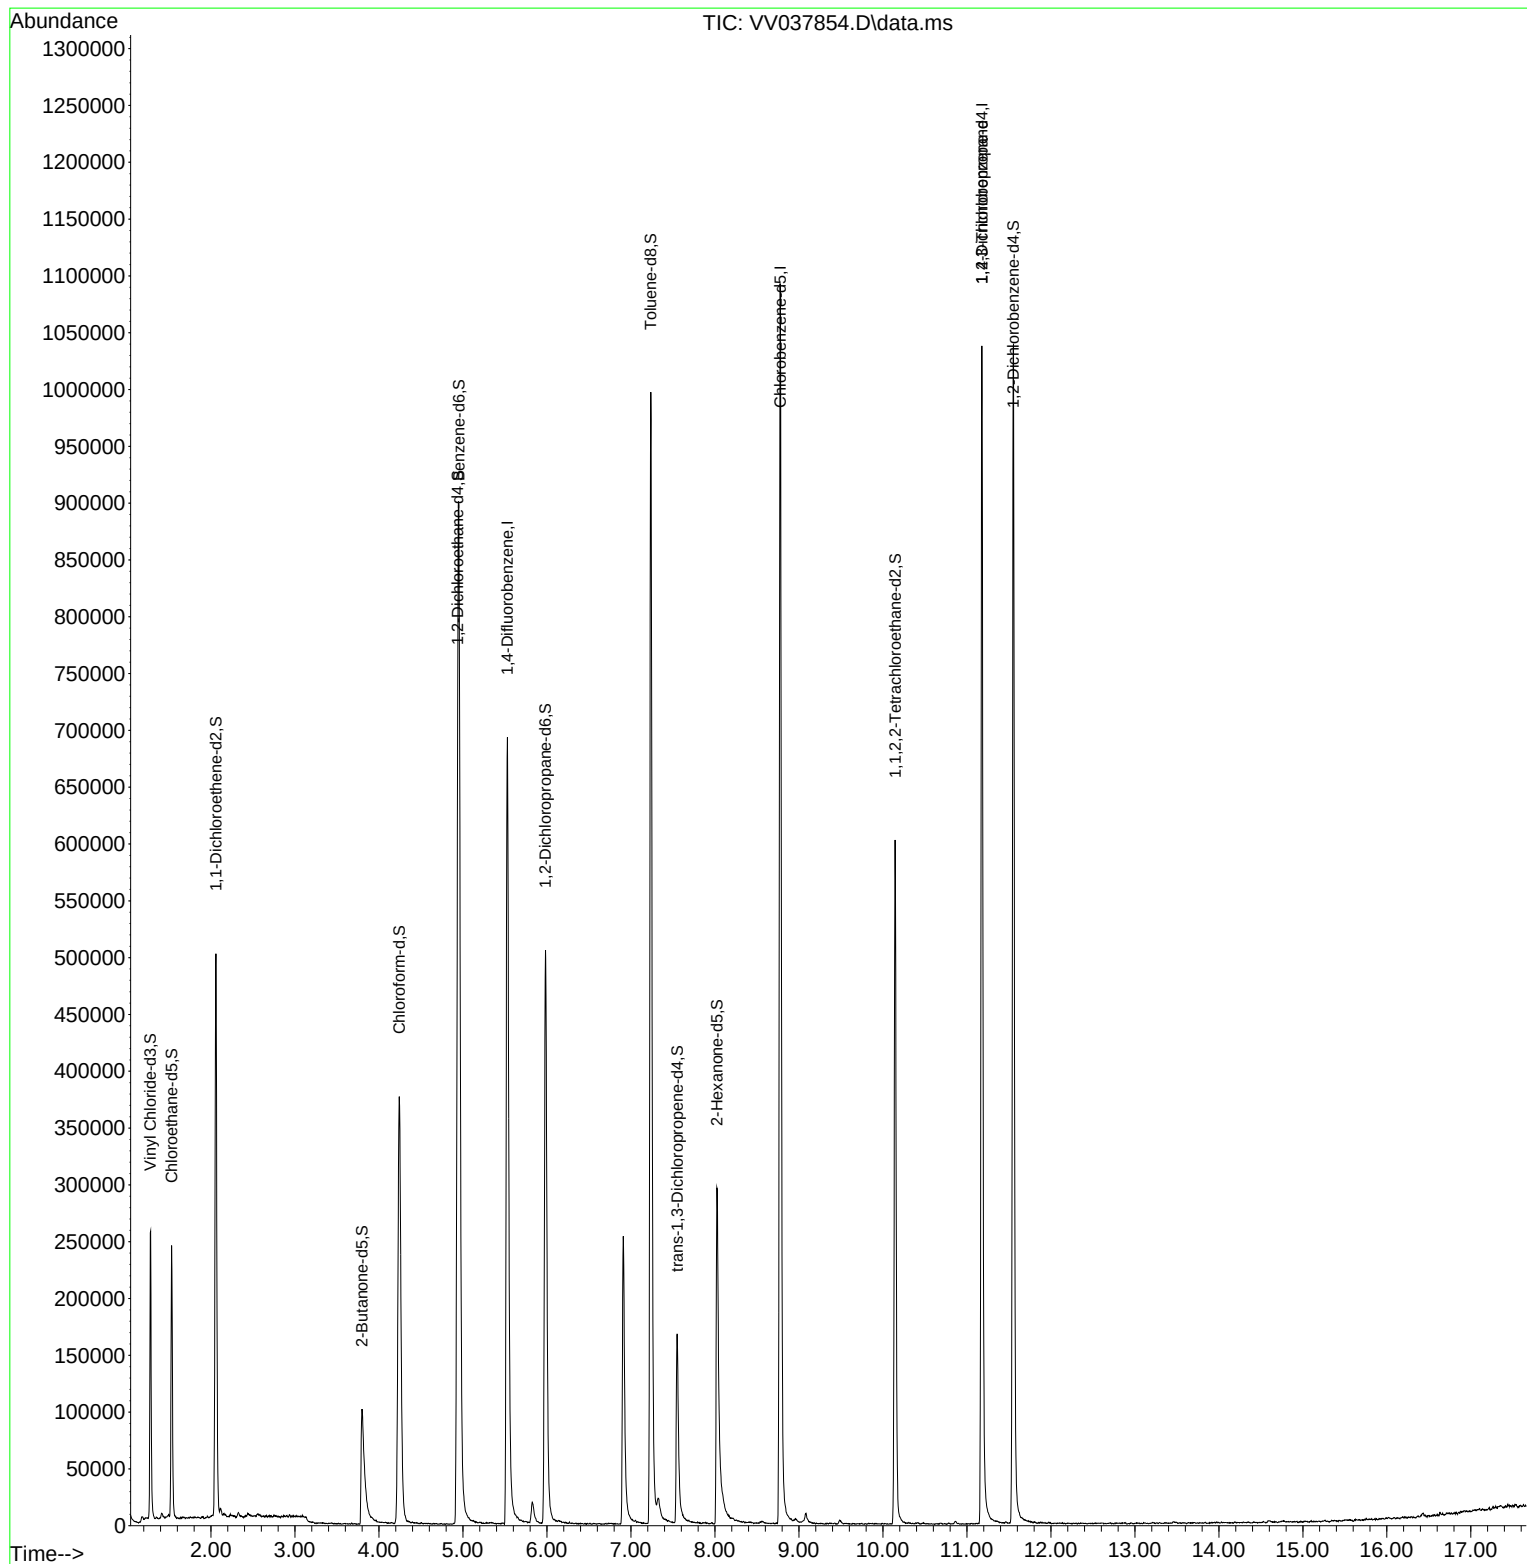

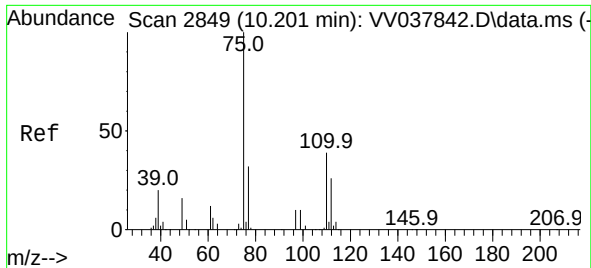

#61

1,2,3-Trichloropropane

Concen: 7.970 ug/L

RT: 11.178 min Scan# 311

Delta R.T. 0.978 min


Lab File: VV037854.D

Acq: 14 Oct 2024 14:12

Instrument :

MSVOA_V

ClientSampleId :

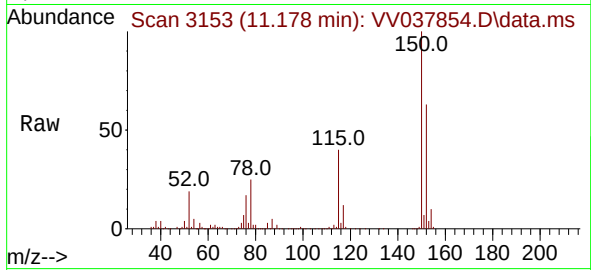

Tgt Ion: 75 Resp: 31183

Ion Ratio Lower Upper

75 100

77 36.5 25.4 38.0

110 2.8 31.7 47.5#

