

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037856.D
 Acq On : 14 Oct 2024 15:00
 Operator : SY/MD
 Sample : P4379-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 15 02:23:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 15 02:19:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	629652	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	630823	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	284047	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	173698	31.425	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	62.860%		
7) Chloroethane-d5	1.532	69	160862	37.494	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	74.980%		
11) 1,1-Dichloroethene-d2	2.056	65	84591	36.631	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.260%		
21) 2-Butanone-d5	3.796	46	159568	81.051	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	81.050%		
24) Chloroform-d	4.239	84	415926	42.296	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.600%		
26) 1,2-Dichloroethane-d4	4.934	65	253755	44.085	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.180%		
32) Benzene-d6	4.950	84	800571	40.556	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.120%		
36) 1,2-Dichloropropane-d6	5.982	67	258478	41.122	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	82.240%		
41) Toluene-d8	7.236	98	697636	38.975	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	77.960%#		
43) trans-1,3-Dichloroprop...	7.548	79	109937	37.650	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.300%		
47) 2-Hexanone-d5	8.024	63	100862	75.991	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	75.990%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	298075	40.812	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.620%		
66) 1,2-Dichlorobenzene-d4	11.554	152	282292	47.163	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.320%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.905	75	6785	0.865	ug/L	# 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037856.D
Acq On : 14 Oct 2024 15:00
Operator : SY/MD
Sample : P4379-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 15 02:23:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 15 02:19:17 2024
Response via : Initial Calibration

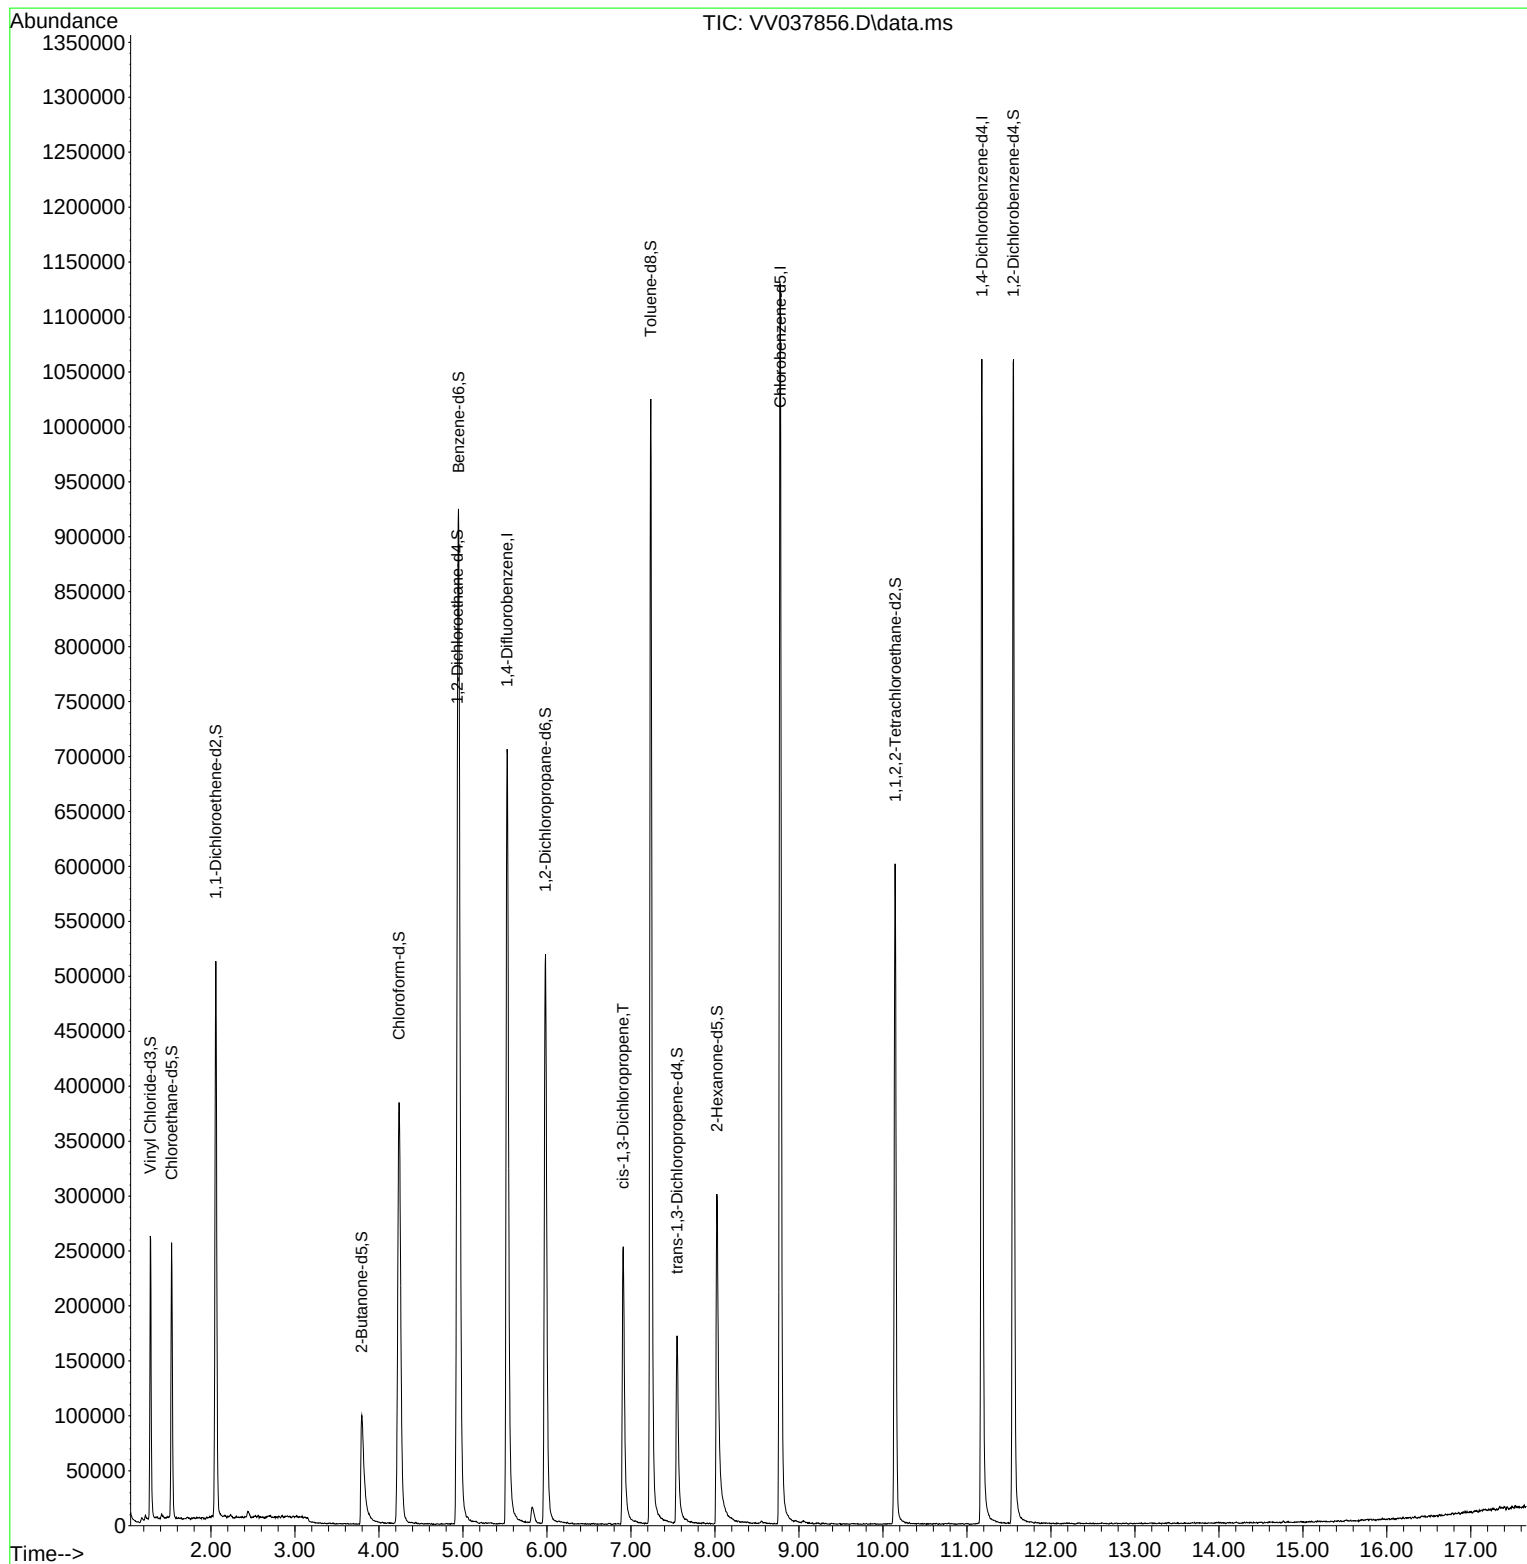

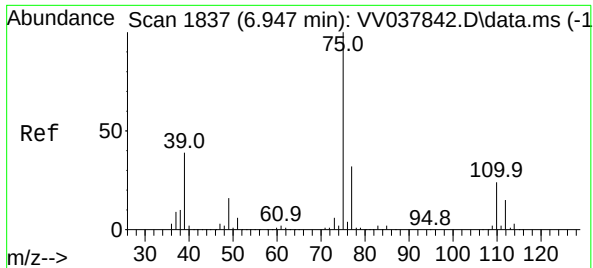

#39
cis-1,3-Dichloropropene
Concen: 0.865 ug/L
RT: 6.905 min Scan# 11
Delta R.T. -0.042 min
Lab File: VV037856.D
Acq: 14 Oct 2024 15:00

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 6785
Ion Ratio Lower Upper
75 100
77 52.7 21.8 40.4#

