

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037844.D
 Acq On : 14 Oct 2024 10:12
 Operator : SY/MD
 Sample : VV1014WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK243

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037844.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	40	43	44	rBV	1586	954	0.04%	0.006%
2	1.220	52	56	58	rBV3	2878	2477	0.11%	0.015%
3	1.281	68	75	89	rVB	259881	280640	12.06%	1.657%
4	1.532	146	153	174	rVB	245208	299239	12.86%	1.767%
5	2.060	307	317	337	rVB	500473	723139	31.07%	4.271%
6	3.204	671	673	676	rBV4	901	505	0.02%	0.003%
7	3.416	736	739	745	rVB5	811	831	0.04%	0.005%
8	3.481	755	759	764	rBV4	832	803	0.03%	0.005%
9	3.744	840	841	848	rVB2	703	601	0.03%	0.004%
10	3.799	849	858	891	rBV2	119287	362994	15.60%	2.144%
11	4.243	980	996	1022	rBV	388505	987010	42.40%	5.829%
12	4.468	1063	1066	1070	rVB3	808	687	0.03%	0.004%
13	4.548	1086	1091	1093	rVV3	839	656	0.03%	0.004%
14	4.577	1096	1100	1104	rVB5	873	788	0.03%	0.005%
15	4.606	1104	1109	1112	rVB4	705	679	0.03%	0.004%
16	4.629	1112	1116	1120	rBV3	963	788	0.03%	0.005%
17	4.696	1133	1137	1142	rVB5	913	886	0.04%	0.005%
18	4.735	1142	1149	1155	rBV4	824	881	0.04%	0.005%
19	4.777	1157	1162	1165	rBV3	1066	817	0.04%	0.005%
20	4.854	1183	1186	1189	rBV2	793	509	0.02%	0.003%
21	4.947	1200	1215	1249	rBV2	928415	2327618	100.00%	13.746%
22	5.281	1317	1319	1324	rVB4	1112	716	0.03%	0.004%
23	5.304	1324	1326	1328	rBV3	1039	541	0.02%	0.003%
24	5.529	1384	1396	1430	rBV	638095	1333087	57.27%	7.873%
25	5.828	1475	1489	1506	rBV4	15913	37326	1.60%	0.220%
26	5.982	1525	1537	1567	rBV	522732	1093905	47.00%	6.460%
27	6.214	1607	1609	1612	rVB3	1549	842	0.04%	0.005%
28	6.239	1612	1617	1619	rVB6	823	733	0.03%	0.004%
29	6.256	1619	1622	1625	rBV4	1037	583	0.03%	0.003%
30	6.313	1635	1640	1642	rBV3	1357	1065	0.05%	0.006%
31	6.326	1642	1644	1648	rVB4	801	527	0.02%	0.003%
32	6.358	1650	1654	1657	rVB5	753	496	0.02%	0.003%
33	6.477	1688	1691	1694	rBV3	656	480	0.02%	0.003%
34	6.526	1700	1706	1711	rBV5	716	704	0.03%	0.004%
35	6.551	1711	1714	1719	rVB4	848	785	0.03%	0.005%
36	6.580	1719	1723	1728	rBV4	785	918	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037844.D
 Acq On : 14 Oct 2024 10:12
 Operator : SY/MD
 Sample : VV1014WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK243

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.641	1739	1742	1745	rBV4	623	601	0.03%	0.004%
38	6.699	1758	1760	1763	rVV2	672	463	0.02%	0.003%
39	6.780	1783	1785	1790	rVB4	805	474	0.02%	0.003%
40	6.908	1815	1825	1856	rBV	251187	498836	21.43%	2.946%
41	7.162	1901	1904	1909	rBV6	921	1002	0.04%	0.006%
42	7.236	1916	1927	1960	rBV	994839	1782209	76.57%	10.525%
43	7.551	2016	2025	2048	rBV	170133	324029	13.92%	1.914%
44	7.809	2102	2105	2106	rBV2	810	516	0.02%	0.003%
45	7.850	2115	2118	2123	rBV5	1055	1009	0.04%	0.006%
46	8.024	2164	2172	2205	rBV2	344263	740889	31.83%	4.375%
47	8.265	2245	2247	2249	rBV2	1223	525	0.02%	0.003%
48	8.548	2325	2335	2337	rBV6	2243	2996	0.13%	0.018%
49	8.657	2365	2369	2373	rVB5	1150	966	0.04%	0.006%
50	8.680	2373	2376	2379	rBV4	1102	924	0.04%	0.005%
51	8.776	2395	2406	2438	rBV	1008446	1694842	72.81%	10.009%
52	9.378	2590	2593	2595	rBV2	729	467	0.02%	0.003%
53	9.448	2609	2615	2618	rBV5	726	790	0.03%	0.005%
54	9.571	2648	2653	2656	rBV5	807	797	0.03%	0.005%
55	9.661	2676	2681	2683	rBV3	693	653	0.03%	0.004%
56	9.802	2722	2725	2727	rBV3	771	501	0.02%	0.003%
57	9.915	2756	2760	2772	rVB5	1120	1742	0.07%	0.010%
58	10.072	2807	2809	2813	rBV2	1008	616	0.03%	0.004%
59	10.146	2820	2832	2856	rBV	665637	1061591	45.61%	6.269%
60	10.403	2910	2912	2916	rBV3	651	488	0.02%	0.003%
61	10.439	2921	2923	2927	rVB4	811	531	0.02%	0.003%
62	10.564	2955	2962	2965	rBV5	742	962	0.04%	0.006%
63	10.760	3020	3023	3027	rBV5	894	701	0.03%	0.004%
64	10.857	3044	3053	3054	rBV3	1067	1416	0.06%	0.008%
65	10.905	3065	3068	3073	rBV4	837	686	0.03%	0.004%
66	10.927	3073	3075	3078	rVB3	860	508	0.02%	0.003%
67	11.085	3120	3124	3128	rBV5	469	542	0.02%	0.003%
68	11.133	3131	3139	3142	rBV5	2242	3146	0.14%	0.019%
69	11.178	3142	3153	3189	rVV	977187	1572980	67.58%	9.290%
70	11.381	3213	3216	3221	rVB6	710	611	0.03%	0.004%
71	11.554	3257	3270	3298	rBV	1070152	1723536	74.05%	10.179%
72	11.824	3351	3354	3357	rBV5	860	775	0.03%	0.005%
73	11.953	3391	3394	3398	rBV4	594	474	0.02%	0.003%
74	12.059	3423	3427	3433	rBV4	705	783	0.03%	0.005%
75	12.194	3465	3469	3471	rBV3	820	558	0.02%	0.003%
76	12.268	3489	3492	3494	rBV2	1071	528	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037844.D
 Acq On : 14 Oct 2024 10:12
 Operator : SY/MD
 Sample : VV1014WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK243

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.545	3572	3578	3582	rBV4	647	648	0.03%	0.004%
78	12.789	3651	3654	3658	rVV5	837	650	0.03%	0.004%
79	12.808	3658	3660	3667	rVB4	892	679	0.03%	0.004%
80	12.943	3700	3702	3705	rVV2	731	485	0.02%	0.003%
81	12.966	3705	3709	3713	rVV5	948	895	0.04%	0.005%
82	12.985	3713	3715	3718	rVV3	915	462	0.02%	0.003%
83	13.069	3733	3741	3745	rBV4	867	1480	0.06%	0.009%
84	13.210	3773	3785	3788	rBV8	3318	5095	0.22%	0.030%
85	13.323	3817	3820	3826	rBV3	817	800	0.03%	0.005%
86	13.352	3826	3829	3832	rBV3	855	713	0.03%	0.004%
87	13.406	3842	3846	3849	rBV4	888	607	0.03%	0.004%
88	13.451	3850	3860	3872	rBV3	5699	12343	0.53%	0.073%
89	13.635	3915	3917	3920	rVB3	990	491	0.02%	0.003%
90	13.689	3925	3934	3940	rVV10	3153	5469	0.23%	0.032%
91	13.747	3950	3952	3956	rVB3	628	462	0.02%	0.003%
92	13.975	4018	4023	4032	rVB5	1576	2613	0.11%	0.015%
93	14.027	4037	4039	4043	rVB2	1089	556	0.02%	0.003%
94	14.127	4065	4070	4072	rBV4	1129	750	0.03%	0.004%
95	14.201	4091	4093	4096	rBV4	1002	689	0.03%	0.004%
96	14.345	4136	4138	4144	rVB7	1077	956	0.04%	0.006%
97	14.387	4147	4151	4152	rBV2	949	544	0.02%	0.003%
98	14.429	4161	4164	4169	rVB4	885	698	0.03%	0.004%
99	14.657	4233	4235	4237	rBV	1601	634	0.03%	0.004%
100	14.725	4252	4256	4260	rVB6	1326	1105	0.05%	0.007%




Sum of corrected areas: 16932697

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037844.D
Acq On : 14 Oct 2024 10:12
Operator : SY/MD
Sample : VV1014WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK243

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

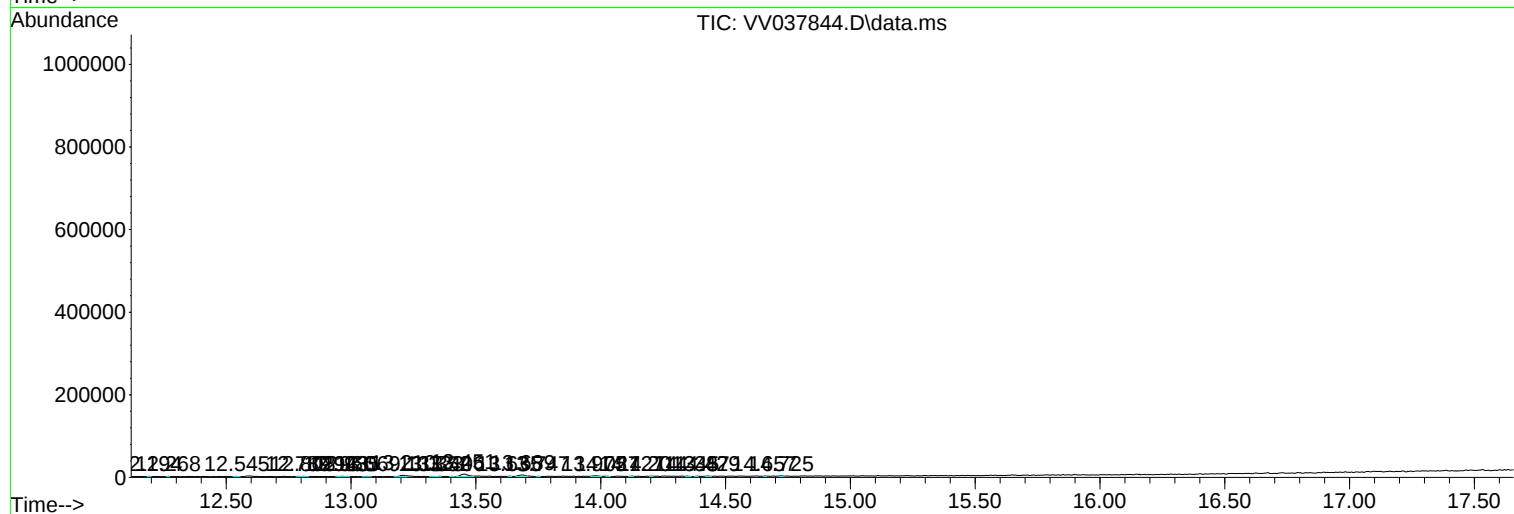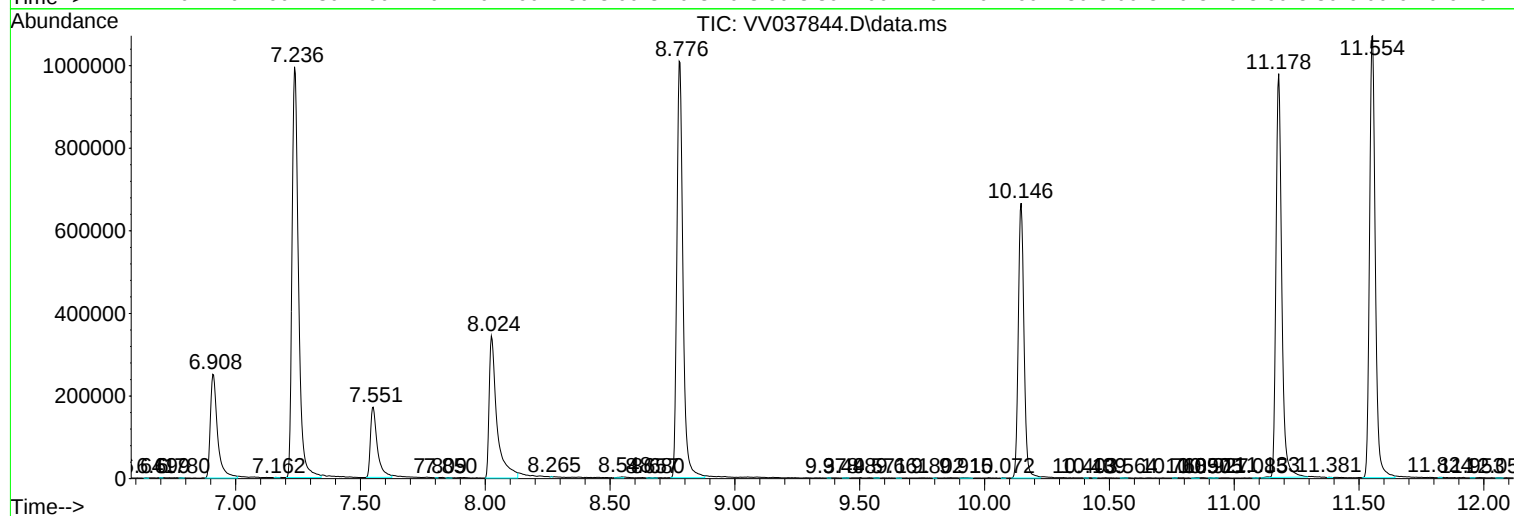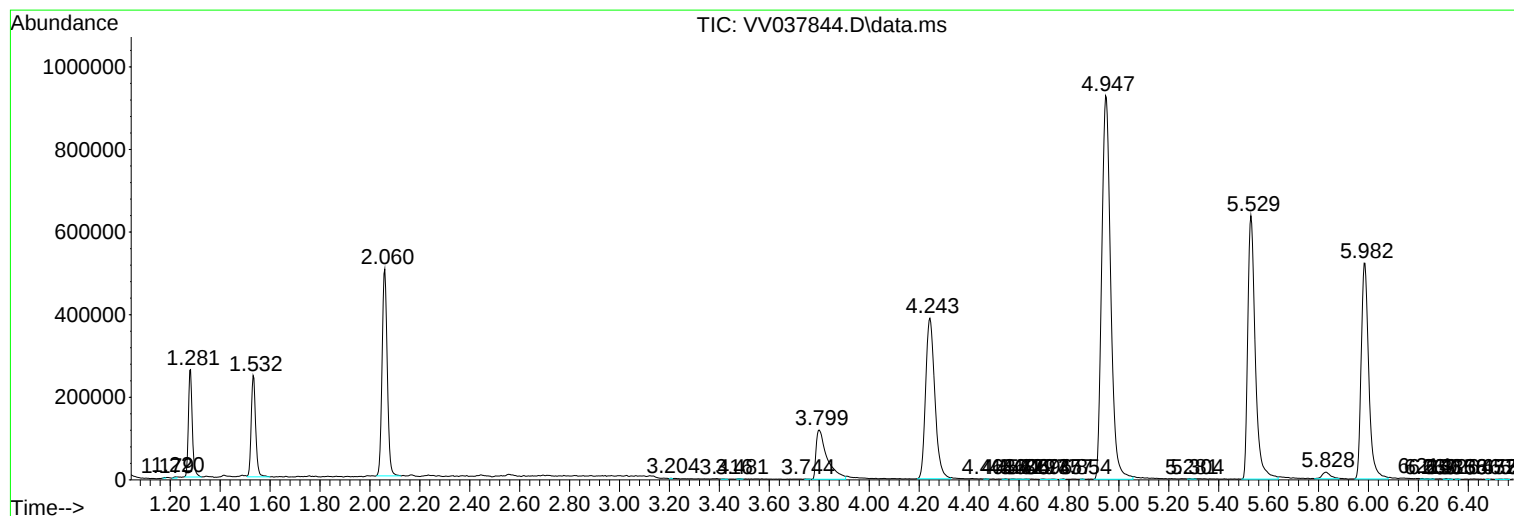

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037844.D
Acq On : 14 Oct 2024 10:12
Operator : SY/MD
Sample : VV1014WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK243

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037844.D
Acq On : 14 Oct 2024 10:12
Operator : SY/MD
Sample : VV1014WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK243

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc