

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037845.D
 Acq On : 14 Oct 2024 10:43
 Operator : SY/MD
 Sample : P4360-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	244823	265660	11.72%	1.604%
2	1.532	146	153	168	rVB	241462	286686	12.65%	1.731%
3	2.056	308	316	331	rVB	481931	694030	30.62%	4.190%
4	3.429	739	743	746	rBV3	949	781	0.03%	0.005%
5	3.532	772	775	776	rBV2	488	250	0.01%	0.002%
6	3.571	785	787	792	rVB4	793	522	0.02%	0.003%
7	3.606	797	798	799	rBV	591	169	0.01%	0.001%
8	3.645	807	810	815	rBV4	408	341	0.02%	0.002%
9	3.693	822	825	827	rBV3	529	345	0.02%	0.002%
10	3.728	833	836	837	rBV2	519	299	0.01%	0.002%
11	3.796	849	857	891	rBV	112274	329043	14.52%	1.987%
12	4.240	979	995	1023	rBV2	382416	973823	42.97%	5.879%
13	4.465	1063	1065	1066	rBV2	680	282	0.01%	0.002%
14	4.677	1128	1131	1136	rVB3	780	761	0.03%	0.005%
15	4.709	1136	1141	1145	rBV3	712	687	0.03%	0.004%
16	4.735	1145	1149	1151	rBV3	559	463	0.02%	0.003%
17	4.767	1157	1159	1162	rBV	374	187	0.01%	0.001%
18	4.854	1180	1186	1189	rVB3	565	569	0.03%	0.003%
19	4.886	1189	1196	1197	rBV4	514	463	0.02%	0.003%
20	4.947	1199	1215	1245	rBV2	900839	2266409	100.00%	13.683%
21	5.285	1318	1320	1323	rBV3	1101	521	0.02%	0.003%
22	5.461	1373	1375	1377	rBV2	750	344	0.02%	0.002%
23	5.526	1384	1395	1423	rBV	646753	1338873	59.07%	8.083%
24	5.760	1465	1468	1472	rBV4	1015	869	0.04%	0.005%
25	5.982	1524	1537	1573	rBV	511625	1071241	47.27%	6.468%
26	6.352	1649	1652	1654	rBV2	1064	638	0.03%	0.004%
27	6.445	1679	1681	1682	rBV	374	201	0.01%	0.001%
28	6.468	1686	1688	1690	rVV4	646	320	0.01%	0.002%
29	6.494	1694	1696	1701	rVB2	370	316	0.01%	0.002%
30	6.522	1701	1705	1706	rBV3	391	313	0.01%	0.002%
31	6.587	1723	1725	1730	rVB3	1056	768	0.03%	0.005%
32	6.609	1730	1732	1734	rBV	268	101	0.00%	0.001%
33	6.625	1734	1737	1739	rBV2	548	347	0.02%	0.002%
34	6.654	1744	1746	1749	rBV2	716	363	0.02%	0.002%
35	6.677	1749	1753	1756	rVB4	800	602	0.03%	0.004%
36	6.715	1756	1765	1767	rBV6	1280	1379	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037845.D
 Acq On : 14 Oct 2024 10:43
 Operator : SY/MD
 Sample : P4360-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.748	1773	1775	1776	rVB3	481	106	0.00%	0.001%
38	6.831	1797	1801	1804	rBV4	789	766	0.03%	0.005%
39	6.847	1804	1806	1810	rVB3	656	378	0.02%	0.002%
40	6.908	1814	1825	1857	rBV	249052	491909	21.70%	2.970%
41	7.194	1910	1914	1916	rBV2	862	656	0.03%	0.004%
42	7.236	1916	1927	1958	rBV	964640	1726909	76.20%	10.426%
43	7.548	2016	2024	2058	rBV	171102	329847	14.55%	1.991%
44	7.992	2157	2162	2163	rBV2	779	665	0.03%	0.004%
45	8.024	2163	2172	2219	rBV2	317875	727154	32.08%	4.390%
46	8.558	2328	2338	2346	rBV8	2311	4724	0.21%	0.029%
47	8.776	2395	2406	2436	rBV	1019520	1714217	75.64%	10.349%
48	9.159	2522	2525	2528	rVB3	705	495	0.02%	0.003%
49	9.175	2528	2530	2535	rVV4	1033	709	0.03%	0.004%
50	9.198	2535	2537	2541	rVB4	562	254	0.01%	0.002%
51	9.278	2560	2562	2564	rBV3	937	521	0.02%	0.003%
52	9.371	2589	2591	2594	rVB2	472	207	0.01%	0.001%
53	9.493	2627	2629	2633	rVB2	456	259	0.01%	0.002%
54	9.542	2642	2644	2645	rBV2	488	183	0.01%	0.001%
55	9.587	2654	2658	2660	rBV2	916	569	0.03%	0.003%
56	9.622	2665	2669	2673	rVV3	610	518	0.02%	0.003%
57	9.670	2682	2684	2691	rVB4	808	730	0.03%	0.004%
58	9.712	2691	2697	2698	rBV2	635	464	0.02%	0.003%
59	9.773	2714	2716	2717	rBV	343	116	0.01%	0.001%
60	9.834	2732	2735	2739	rBV3	611	466	0.02%	0.003%
61	9.921	2760	2762	2769	rBV2	705	543	0.02%	0.003%
62	9.950	2769	2771	2778	rVB5	861	736	0.03%	0.004%
63	9.989	2778	2783	2784	rBV3	420	403	0.02%	0.002%
64	10.069	2806	2808	2810	rVB	503	193	0.01%	0.001%
65	10.091	2812	2815	2818	rBV3	460	331	0.01%	0.002%
66	10.146	2820	2832	2855	rBV	637987	1030523	45.47%	6.222%
67	10.320	2880	2886	2894	rVB5	3226	4959	0.22%	0.030%
68	10.484	2932	2937	2938	rBV2	947	721	0.03%	0.004%
69	10.532	2950	2952	2953	rBV	388	148	0.01%	0.001%
70	10.590	2968	2970	2971	rBV2	656	243	0.01%	0.001%
71	10.767	3023	3025	3027	rBV	365	128	0.01%	0.001%
72	10.780	3027	3029	3031	rBV2	580	278	0.01%	0.002%
73	10.821	3040	3042	3044	rVB2	564	274	0.01%	0.002%
74	10.844	3044	3049	3051	rBV2	750	572	0.03%	0.003%
75	10.889	3062	3063	3065	rVB	545	118	0.01%	0.001%
76	10.979	3087	3091	3093	rBV2	698	514	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037845.D
Acq On : 14 Oct 2024 10:43
Operator : SY/MD
Sample : P4360-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

77	11.021	3101	3104	3105	rBV	266	148	0.01%	0.001%
78	11.178	3143	3153	3185	rBV	985998	1593432	70.31%	9.620%
79	11.551	3258	3269	3298	rBV	1038069	1683077	74.26%	10.161%
80	11.921	3382	3384	3387	rBV4	795	369	0.02%	0.002%
81	12.294	3498	3500	3502	rVB	658	243	0.01%	0.001%
82	12.316	3502	3507	3509	rBV4	974	871	0.04%	0.005%
83	12.580	3587	3589	3592	rBV3	785	672	0.03%	0.004%
84	12.805	3657	3659	3662	rBV	474	211	0.01%	0.001%
85	13.050	3733	3735	3738	rBV3	717	351	0.02%	0.002%
86	13.101	3749	3751	3754	rBV	427	316	0.01%	0.002%
87	13.191	3776	3779	3780	rBV2	726	446	0.02%	0.003%
88	13.281	3805	3807	3809	rBV3	798	371	0.02%	0.002%
89	14.422	4160	4162	4164	rBV4	833	401	0.02%	0.002%




Sum of corrected areas: 16563380

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037845.D
Acq On : 14 Oct 2024 10:43
Operator : SY/MD
Sample : P4360-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

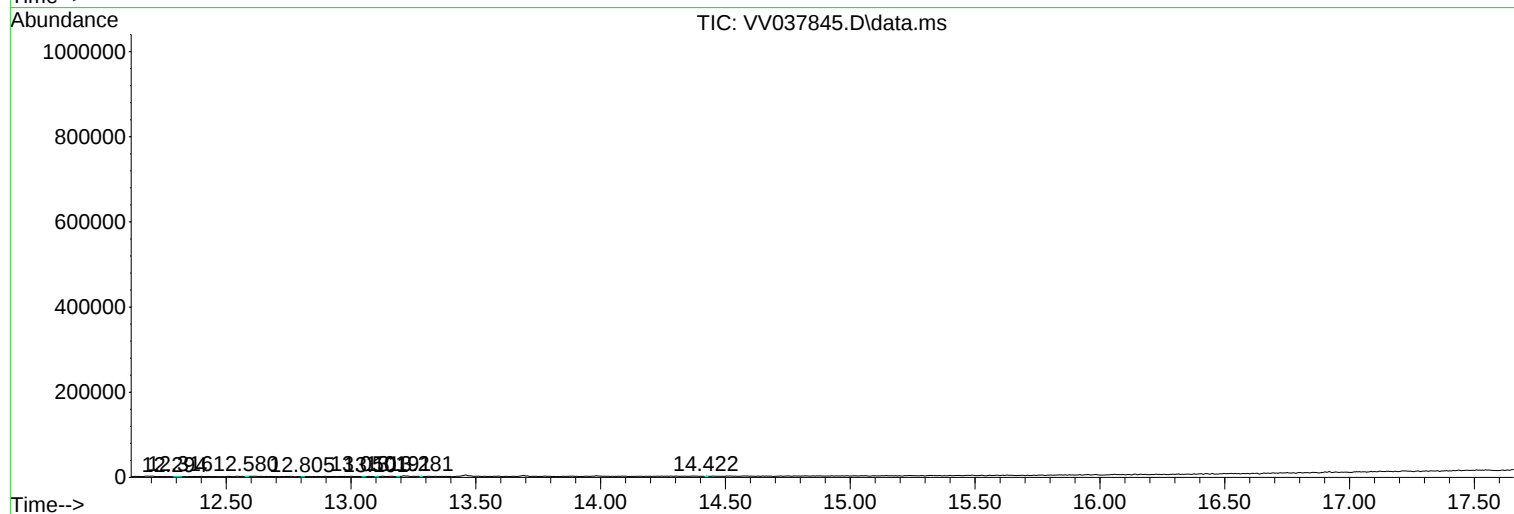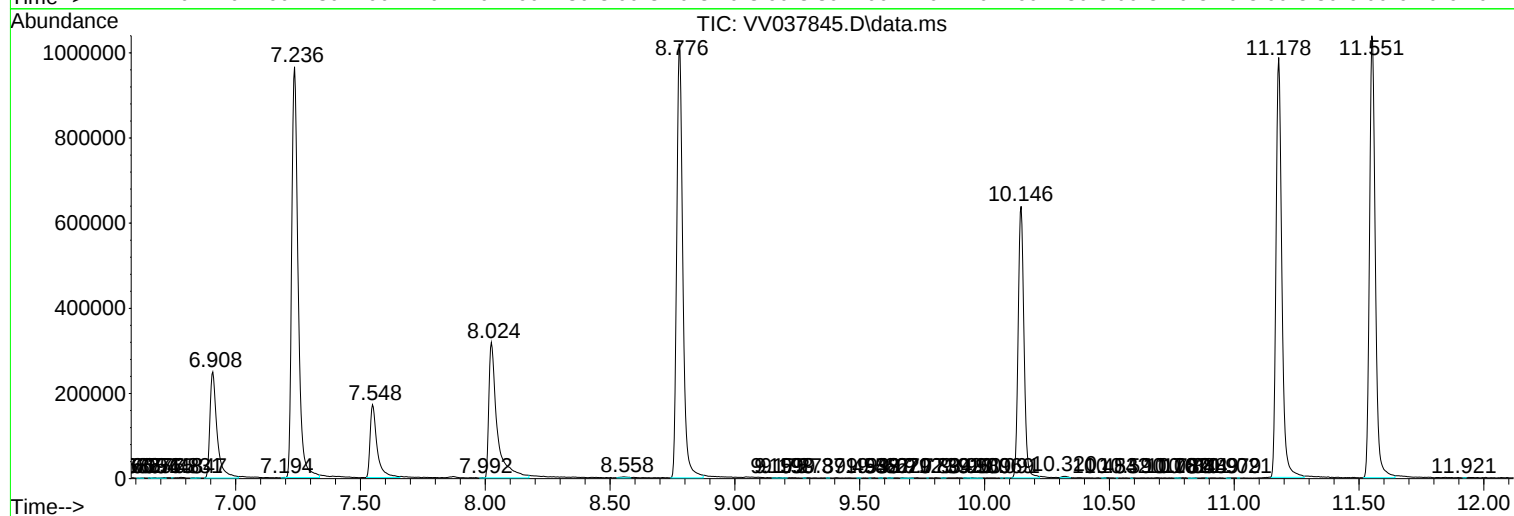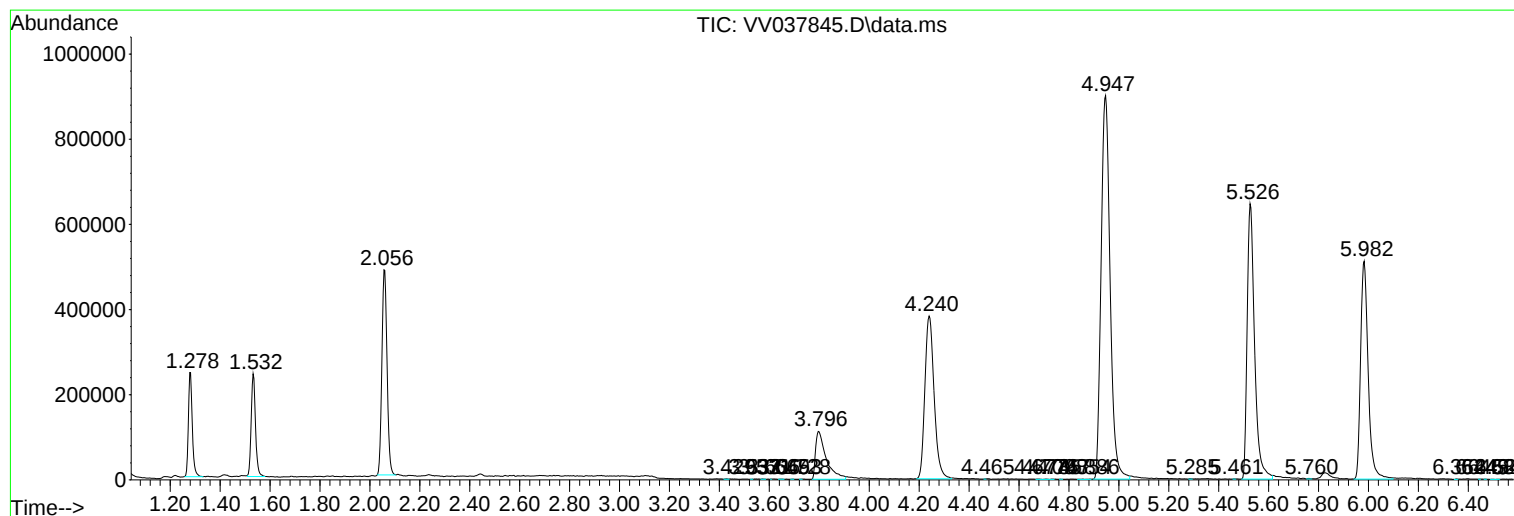

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037845.D
Acq On : 14 Oct 2024 10:43
Operator : SY/MD
Sample : P4360-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037845.D
Acq On : 14 Oct 2024 10:43
Operator : SY/MD
Sample : P4360-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------