

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037847.D
 Acq On : 14 Oct 2024 11:26
 Operator : SY/MD
 Sample : P4352-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	51	rBV2	4260	7442	0.31%	0.043%
2	1.282	68	75	88	rVB	264029	278535	11.58%	1.606%
3	1.536	146	154	167	rVB	252012	300112	12.47%	1.730%
4	2.060	307	317	331	rBV	516501	742378	30.85%	4.279%
5	3.198	668	671	673	rBV3	849	584	0.02%	0.003%
6	3.278	692	696	699	rVB4	1120	762	0.03%	0.004%
7	3.593	790	794	798	rBV4	677	548	0.02%	0.003%
8	3.799	847	858	896	rBV	122569	354308	14.72%	2.042%
9	4.175	972	975	978	rBV4	720	495	0.02%	0.003%
10	4.243	979	996	1025	rBV	400967	1027114	42.69%	5.921%
11	4.645	1117	1121	1124	rBV5	563	466	0.02%	0.003%
12	4.741	1147	1151	1155	rBV4	849	913	0.04%	0.005%
13	4.950	1201	1216	1252	rBV2	959454	2406190	100.00%	13.870%
14	5.224	1299	1301	1304	rVB2	1039	571	0.02%	0.003%
15	5.333	1333	1335	1338	rBV3	710	462	0.02%	0.003%
16	5.404	1355	1357	1361	rVB3	1198	832	0.03%	0.005%
17	5.461	1372	1375	1379	rBV4	601	556	0.02%	0.003%
18	5.529	1382	1396	1430	rBV	645848	1350325	56.12%	7.784%
19	5.825	1479	1488	1489	rBV2	15343	15293	0.64%	0.088%
20	5.986	1525	1538	1571	rBV	548563	1143514	47.52%	6.592%
21	6.262	1622	1624	1627	rVB3	960	518	0.02%	0.003%
22	6.330	1639	1645	1648	rVB7	856	907	0.04%	0.005%
23	6.349	1648	1651	1654	rVB	643	449	0.02%	0.003%
24	6.410	1668	1670	1674	rVB4	722	469	0.02%	0.003%
25	6.487	1691	1694	1699	rVB3	839	780	0.03%	0.004%
26	6.529	1704	1707	1713	rVB4	1311	1102	0.05%	0.006%
27	6.651	1741	1745	1748	rBV4	924	841	0.03%	0.005%
28	6.728	1763	1769	1771	rBV5	1307	1238	0.05%	0.007%
29	6.748	1773	1775	1779	rBV4	644	473	0.02%	0.003%
30	6.815	1790	1796	1798	rBV2	801	633	0.03%	0.004%
31	6.908	1814	1825	1861	rBV	263334	523328	21.75%	3.017%
32	7.236	1916	1927	1963	rBV	1041150	1844637	76.66%	10.633%
33	7.551	2013	2025	2052	rBV	179871	346519	14.40%	1.997%
34	7.703	2070	2072	2074	rBV2	882	465	0.02%	0.003%
35	7.960	2147	2152	2154	rBV4	1004	975	0.04%	0.006%
36	8.024	2164	2172	2211	rBV2	346503	766780	31.87%	4.420%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037847.D
 Acq On : 14 Oct 2024 11:26
 Operator : SY/MD
 Sample : P4352-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.410	2289	2292	2294	rVB2	850	535	0.02%	0.003%
38	8.548	2329	2335	2336	rBV5	2154	1612	0.07%	0.009%
39	8.645	2362	2365	2368	rBV4	882	485	0.02%	0.003%
40	8.731	2390	2392	2395	rVB4	772	453	0.02%	0.003%
41	8.780	2395	2407	2442	rBV	1025307	1724897	71.69%	9.943%
42	9.153	2520	2523	2525	rBV4	925	625	0.03%	0.004%
43	9.262	2553	2557	2560	rBV5	1035	851	0.04%	0.005%
44	9.284	2560	2564	2568	rVV4	633	566	0.02%	0.003%
45	9.358	2581	2587	2592	rVB5	966	1228	0.05%	0.007%
46	9.403	2597	2601	2606	rVB5	752	941	0.04%	0.005%
47	9.439	2606	2612	2615	rBV5	983	983	0.04%	0.006%
48	9.635	2671	2673	2675	rBV2	686	452	0.02%	0.003%
49	9.674	2681	2685	2690	rVB3	838	690	0.03%	0.004%
50	9.699	2690	2693	2700	rBV3	553	528	0.02%	0.003%
51	9.812	2722	2728	2735	rVB6	632	815	0.03%	0.005%
52	10.146	2819	2832	2858	rBV	694478	1105916	45.96%	6.375%
53	10.329	2888	2889	2894	rVB3	1223	550	0.02%	0.003%
54	10.500	2939	2942	2947	rVB2	871	501	0.02%	0.003%
55	10.622	2976	2980	2982	rBV3	945	547	0.02%	0.003%
56	10.696	2999	3003	3006	rBV3	518	473	0.02%	0.003%
57	10.728	3011	3013	3018	rVB2	911	534	0.02%	0.003%
58	10.786	3028	3031	3034	rVB3	1156	794	0.03%	0.005%
59	10.854	3048	3052	3055	rBV4	548	542	0.02%	0.003%
60	10.879	3056	3060	3064	rVB2	640	530	0.02%	0.003%
61	10.902	3064	3067	3072	rVB2	825	689	0.03%	0.004%
62	10.989	3089	3094	3099	rVB3	664	597	0.02%	0.003%
63	11.056	3114	3115	3123	rVB5	814	729	0.03%	0.004%
64	11.091	3123	3126	3129	rBV4	780	453	0.02%	0.003%
65	11.136	3134	3140	3142	rBV5	1169	1258	0.05%	0.007%
66	11.178	3142	3153	3190	rBV	985701	1572287	65.34%	9.063%
67	11.432	3228	3232	3233	rBV3	840	648	0.03%	0.004%
68	11.554	3258	3270	3294	rBV	1087450	1777234	73.86%	10.245%
69	11.860	3361	3365	3371	rBV4	1023	1495	0.06%	0.009%
70	11.902	3375	3378	3382	rBV4	755	549	0.02%	0.003%
71	12.021	3412	3415	3418	rBV3	989	555	0.02%	0.003%
72	12.178	3460	3464	3465	rBV3	860	503	0.02%	0.003%
73	12.201	3469	3471	3476	rVB3	836	449	0.02%	0.003%
74	12.294	3495	3500	3506	rBV4	652	791	0.03%	0.005%
75	12.509	3565	3567	3571	rVB4	705	469	0.02%	0.003%
76	12.564	3576	3584	3586	rBV5	901	789	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037847.D
 Acq On : 14 Oct 2024 11:26
 Operator : SY/MD
 Sample : P4352-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.590	3588	3592	3596	rBV5	1154	987	0.04%	0.006%
78	12.654	3608	3612	3614	rBV4	625	468	0.02%	0.003%
79	12.693	3620	3624	3629	rBV5	814	622	0.03%	0.004%
80	13.075	3739	3743	3748	rBV4	829	916	0.04%	0.005%
81	13.214	3784	3786	3789	rVV3	698	483	0.02%	0.003%
82	13.281	3806	3807	3811	rVB3	1147	662	0.03%	0.004%
83	13.307	3812	3815	3822	rVB5	750	695	0.03%	0.004%
84	13.368	3831	3834	3838	rVB3	1012	488	0.02%	0.003%
85	13.416	3846	3849	3854	rBV3	775	636	0.03%	0.004%
86	13.461	3859	3863	3865	rBV5	894	746	0.03%	0.004%
87	13.542	3886	3888	3893	rVB3	930	587	0.02%	0.003%
88	13.603	3904	3907	3909	rBV4	901	523	0.02%	0.003%
89	13.689	3931	3934	3942	rVB6	1581	1554	0.06%	0.009%
90	13.834	3976	3979	3981	rBV4	758	503	0.02%	0.003%
91	13.953	4013	4016	4018	rBV2	979	672	0.03%	0.004%
92	13.979	4019	4024	4032	rVV5	2325	3491	0.15%	0.020%
93	14.021	4032	4037	4038	rVV2	1073	713	0.03%	0.004%
94	14.040	4041	4043	4046	rVB2	1093	510	0.02%	0.003%
95	14.082	4052	4056	4058	rBV3	926	645	0.03%	0.004%
96	14.943	4321	4324	4332	rVB6	1363	1471	0.06%	0.008%
97	14.979	4332	4335	4337	rBV4	1158	576	0.02%	0.003%
98	15.223	4407	4411	4414	rBV4	1155	776	0.03%	0.004%
99	15.287	4427	4431	4433	rBV3	1625	1160	0.05%	0.007%
100	15.844	4602	4604	4606	rBV3	1733	1075	0.04%	0.006%




Sum of corrected areas: 17348016

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037847.D
Acq On : 14 Oct 2024 11:26
Operator : SY/MD
Sample : P4352-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

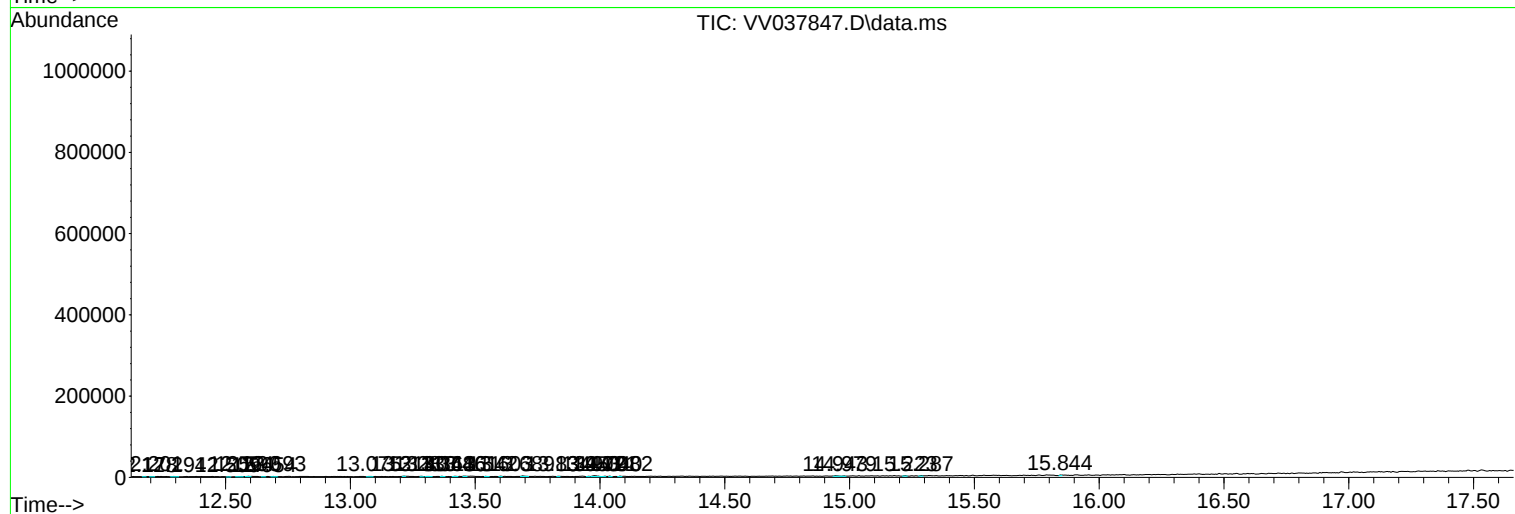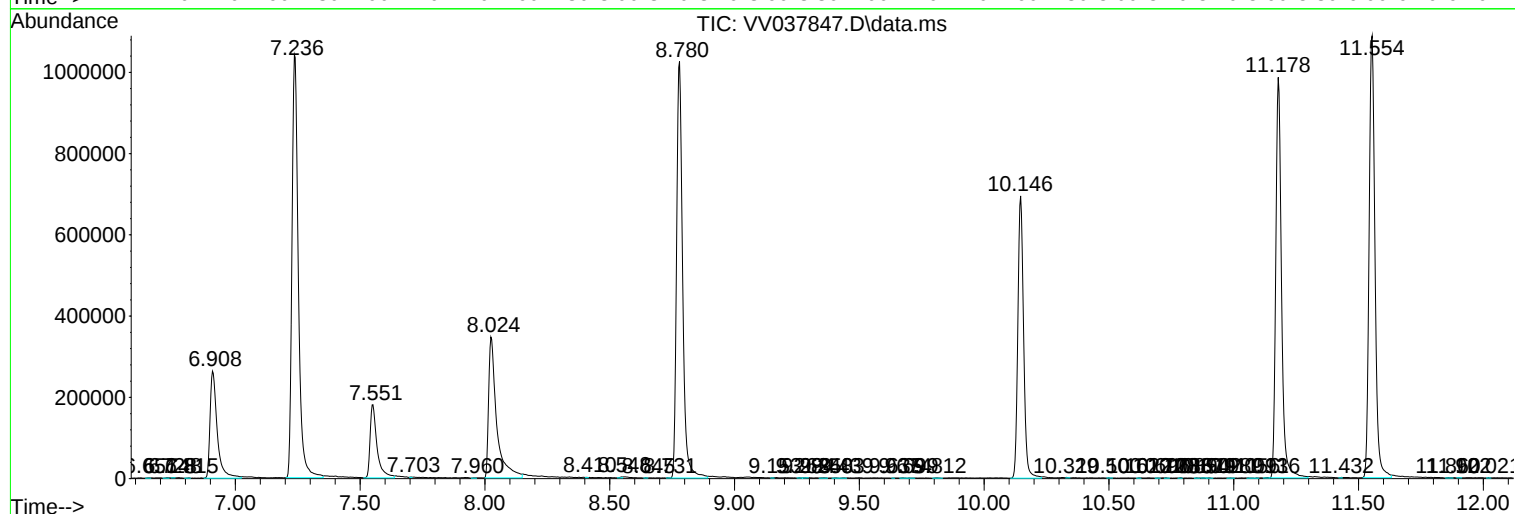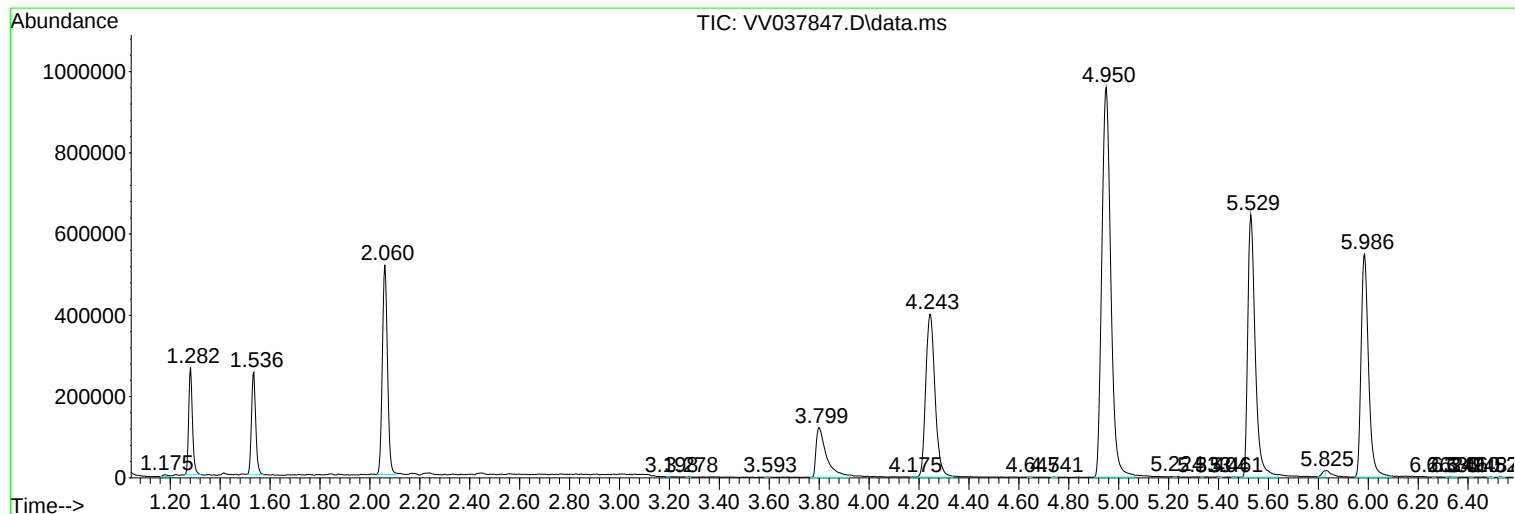

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037847.D
Acq On : 14 Oct 2024 11:26
Operator : SY/MD
Sample : P4352-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037847.D
Acq On : 14 Oct 2024 11:26
Operator : SY/MD
Sample : P4352-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------