

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037848.D
 Acq On : 14 Oct 2024 11:48
 Operator : SY/MD
 Sample : P4349-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rBV	247698	263721	11.35%	1.599%
2	1.532	146	153	170	rVB	244689	285908	12.30%	1.733%
3	2.059	307	317	334	rBV	487078	701087	30.16%	4.251%
4	3.413	736	738	739	rBV	564	176	0.01%	0.001%
5	3.455	748	751	753	rBV3	457	284	0.01%	0.002%
6	3.497	762	764	767	rBV2	605	392	0.02%	0.002%
7	3.529	771	774	775	rBV2	420	210	0.01%	0.001%
8	3.542	775	778	783	rVB4	571	549	0.02%	0.003%
9	3.600	791	796	802	rVB3	795	907	0.04%	0.005%
10	3.683	820	822	823	rBV2	411	173	0.01%	0.001%
11	3.735	835	838	840	rBV4	551	378	0.02%	0.002%
12	3.796	849	857	889	rBV	115505	325461	14.00%	1.973%
13	4.243	981	996	1030	rBV	391007	984636	42.36%	5.970%
14	4.667	1125	1128	1130	rVB2	504	295	0.01%	0.002%
15	4.686	1130	1134	1136	rBV3	509	357	0.02%	0.002%
16	4.773	1158	1161	1162	rBV3	395	211	0.01%	0.001%
17	4.812	1171	1173	1178	rBV2	384	229	0.01%	0.001%
18	4.866	1187	1190	1193	rVB2	534	277	0.01%	0.002%
19	4.883	1193	1195	1196	rBV	435	199	0.01%	0.001%
20	4.950	1201	1216	1258	rBV2	908308	2324468	100.00%	14.093%
21	5.281	1317	1319	1322	rVB2	996	441	0.02%	0.003%
22	5.484	1381	1382	1385	rVB3	545	275	0.01%	0.002%
23	5.529	1385	1396	1433	rBV	608196	1276143	54.90%	7.737%
24	5.985	1525	1538	1573	rBV	516121	1094639	47.09%	6.637%
25	6.432	1673	1677	1678	rBV3	618	373	0.02%	0.002%
26	6.452	1681	1683	1685	rVB2	499	209	0.01%	0.001%
27	6.551	1711	1714	1715	rBV3	649	340	0.01%	0.002%
28	6.561	1715	1717	1721	rVV4	698	530	0.02%	0.003%
29	6.580	1721	1723	1728	rVB3	889	639	0.03%	0.004%
30	6.599	1728	1729	1730	rBV	227	77	0.00%	0.000%
31	6.609	1730	1732	1736	rBV5	728	499	0.02%	0.003%
32	6.644	1741	1743	1745	rVV3	693	343	0.01%	0.002%
33	6.657	1745	1747	1751	rVV2	939	687	0.03%	0.004%
34	6.683	1753	1755	1758	rVB2	766	393	0.02%	0.002%
35	6.802	1789	1792	1795	rBV2	694	477	0.02%	0.003%
36	6.837	1801	1803	1809	rBV2	583	350	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037848.D
 Acq On : 14 Oct 2024 11:48
 Operator : SY/MD
 Sample : P4349-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.908	1815	1825	1860	rBV	253474	497718	21.41%	3.018%
38	7.236	1916	1927	1961	rBV	981670	1766120	75.98%	10.708%
39	7.551	2015	2025	2055	rBV	173043	332717	14.31%	2.017%
40	7.911	2133	2137	2138	rBV4	646	466	0.02%	0.003%
41	7.976	2154	2157	2160	rBV3	897	707	0.03%	0.004%
42	8.024	2164	2172	2217	rBV2	342616	752754	32.38%	4.564%
43	8.702	2379	2383	2390	rVB4	774	760	0.03%	0.005%
44	8.731	2390	2392	2395	rBV2	673	390	0.02%	0.002%
45	8.779	2396	2407	2440	rBV	978137	1632731	70.24%	9.899%
46	9.217	2540	2543	2548	rBV7	901	923	0.04%	0.006%
47	9.259	2554	2556	2559	rVB3	909	443	0.02%	0.003%
48	9.287	2563	2565	2568	rVB2	749	354	0.02%	0.002%
49	9.336	2578	2580	2581	rBV2	339	158	0.01%	0.001%
50	9.378	2589	2593	2596	rBV3	658	579	0.02%	0.004%
51	9.419	2603	2606	2608	rVB	882	527	0.02%	0.003%
52	9.484	2622	2626	2631	rVB6	701	714	0.03%	0.004%
53	9.567	2650	2652	2654	rBV3	428	198	0.01%	0.001%
54	9.677	2684	2686	2690	rVB	562	286	0.01%	0.002%
55	9.699	2690	2693	2694	rBV	381	223	0.01%	0.001%
56	9.773	2713	2716	2718	rBV2	220	177	0.01%	0.001%
57	9.786	2718	2720	2721	rBV	388	169	0.01%	0.001%
58	9.837	2733	2736	2738	rVB2	827	455	0.02%	0.003%
59	9.866	2741	2745	2748	rBV2	411	400	0.02%	0.002%
60	9.921	2760	2762	2767	rBV3	466	251	0.01%	0.002%
61	9.992	2779	2784	2786	rVB2	928	729	0.03%	0.004%
62	10.004	2786	2788	2791	rBV2	576	295	0.01%	0.002%
63	10.024	2791	2794	2795	rBV2	342	204	0.01%	0.001%
64	10.146	2820	2832	2852	rBV	671757	1057707	45.50%	6.413%
65	10.390	2906	2908	2911	rVB2	598	231	0.01%	0.001%
66	10.474	2932	2934	2937	rBV3	654	376	0.02%	0.002%
67	10.516	2944	2947	2950	rVB2	823	516	0.02%	0.003%
68	10.580	2957	2967	2969	rBV2	841	1134	0.05%	0.007%
69	10.651	2984	2989	2990	rBV2	708	511	0.02%	0.003%
70	10.744	3016	3018	3019	rBV	288	120	0.01%	0.001%
71	10.770	3023	3026	3027	rBV	446	270	0.01%	0.002%
72	10.831	3043	3045	3047	rBV	312	137	0.01%	0.001%
73	10.869	3051	3057	3061	rBV4	1032	1192	0.05%	0.007%
74	10.947	3079	3081	3082	rBV2	366	122	0.01%	0.001%
75	10.976	3089	3090	3091	rBV2	386	114	0.00%	0.001%
76	11.078	3119	3122	3124	rBV	341	209	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037848.D
 Acq On : 14 Oct 2024 11:48
 Operator : SY/MD
 Sample : P4349-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

77	11.130	3134	3138	3140	rBV3	1559	1088	0.05%	0.007%
78	11.178	3142	3153	3186	rVV	917710	1476449	63.52%	8.952%
79	11.554	3258	3270	3296	rBV	1038381	1692495	72.81%	10.261%
80	12.181	3463	3465	3469	rBV2	628	322	0.01%	0.002%
81	12.532	3570	3574	3575	rBV2	803	540	0.02%	0.003%
82	12.689	3621	3623	3627	rVB3	576	279	0.01%	0.002%
83	13.213	3782	3786	3789	rBV5	1985	1610	0.07%	0.010%
84	13.297	3810	3812	3815	rBV2	763	456	0.02%	0.003%




Sum of corrected areas: 16493659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037848.D
Acq On : 14 Oct 2024 11:48
Operator : SY/MD
Sample : P4349-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

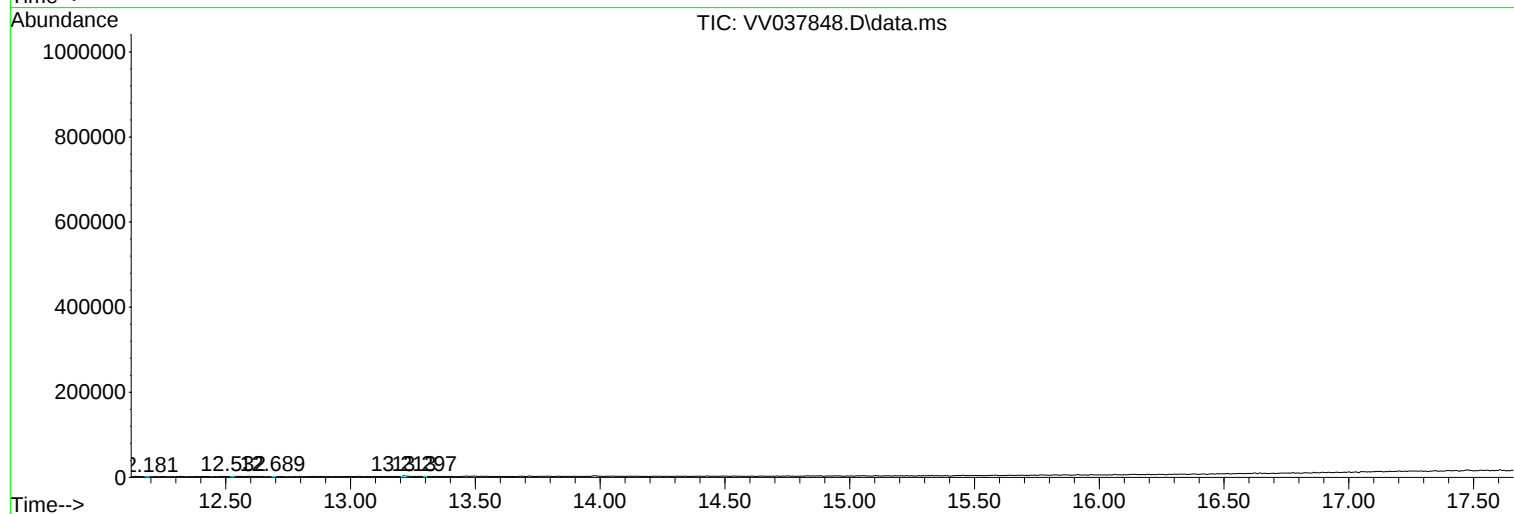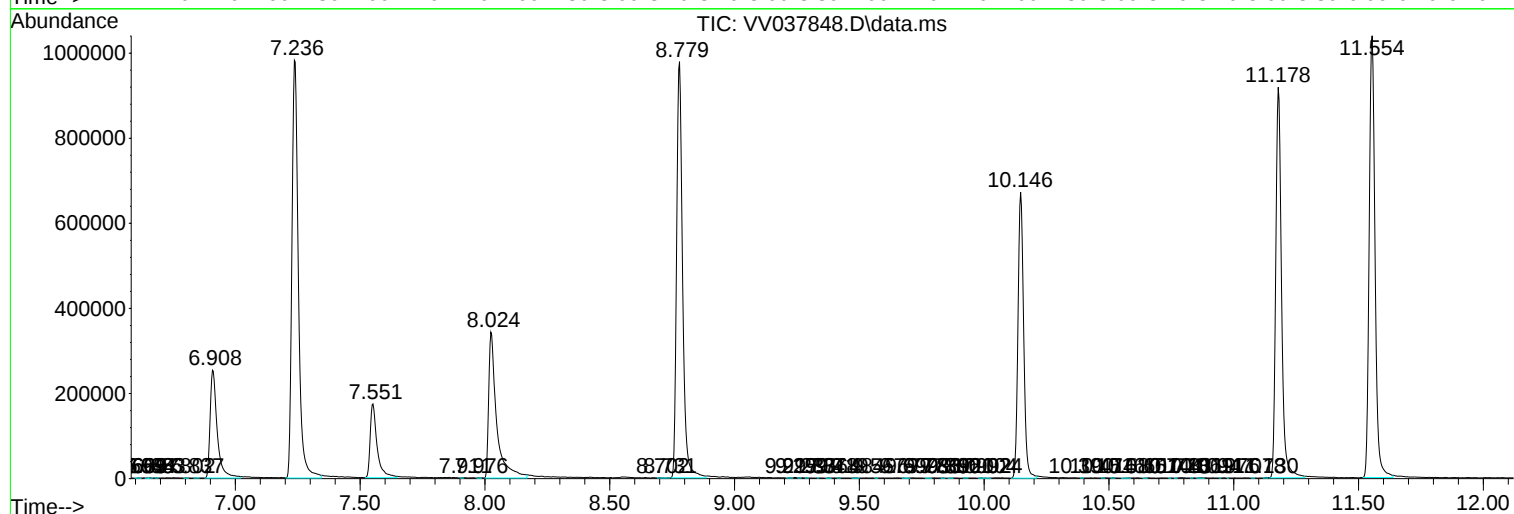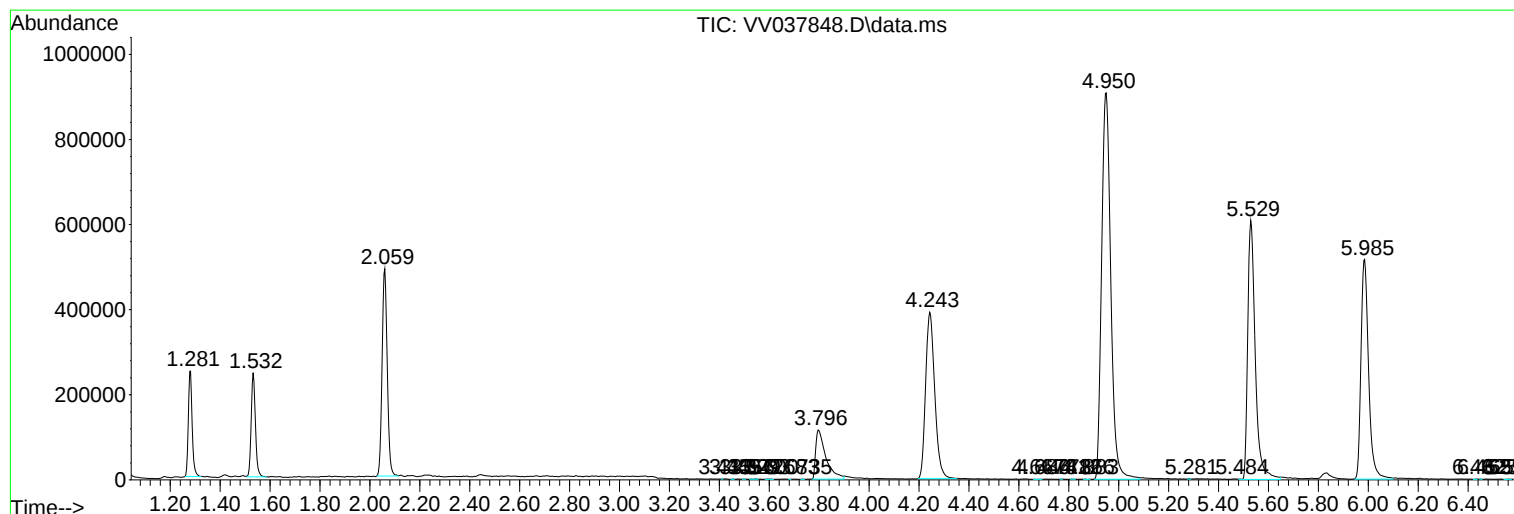

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037848.D
Acq On : 14 Oct 2024 11:48
Operator : SY/MD
Sample : P4349-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037848.D
Acq On : 14 Oct 2024 11:48
Operator : SY/MD
Sample : P4349-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc