

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037851.D
 Acq On : 14 Oct 2024 13:08
 Operator : SY/MD
 Sample : P4379-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	297790	315656	12.41%	1.646%
2	1.532	146	153	170	rVB	266004	321127	12.63%	1.674%
3	2.057	307	316	330	rBV	562338	802516	31.56%	4.185%
4	3.484	758	760	762	rBV	357	150	0.01%	0.001%
5	3.539	774	777	778	rBV2	718	364	0.01%	0.002%
6	3.645	808	810	811	rBV2	531	208	0.01%	0.001%
7	3.680	819	821	822	rBV	426	148	0.01%	0.001%
8	3.700	825	827	829	rVB2	670	255	0.01%	0.001%
9	3.793	845	856	894	rBV	111607	333587	13.12%	1.739%
10	4.240	979	995	1021	rBV	413312	1044048	41.06%	5.444%
11	4.497	1072	1075	1077	rBV2	700	392	0.02%	0.002%
12	4.597	1104	1106	1109	rVB3	771	361	0.01%	0.002%
13	4.658	1122	1125	1129	rVB3	468	311	0.01%	0.002%
14	4.706	1137	1140	1141	rBV2	408	242	0.01%	0.001%
15	4.944	1199	1214	1251	rBV2	1007704	2542778	100.00%	13.259%
16	5.484	1380	1382	1383	rBV	881	284	0.01%	0.001%
17	5.526	1384	1395	1428	rBV	859373	1774863	69.80%	9.255%
18	5.979	1523	1536	1573	rBV	559459	1168924	45.97%	6.095%
19	6.381	1659	1661	1665	rVB4	1098	666	0.03%	0.003%
20	6.420	1670	1673	1675	rBV2	469	282	0.01%	0.001%
21	6.532	1704	1708	1709	rBV2	785	412	0.02%	0.002%
22	6.574	1719	1721	1725	rBV3	816	476	0.02%	0.002%
23	6.597	1727	1728	1729	rBV	399	115	0.00%	0.001%
24	6.629	1736	1738	1742	rBV3	434	278	0.01%	0.001%
25	6.667	1748	1750	1753	rVB2	660	360	0.01%	0.002%
26	6.751	1772	1776	1779	rBV3	685	486	0.02%	0.003%
27	6.767	1779	1781	1784	rVB3	742	423	0.02%	0.002%
28	6.786	1785	1787	1792	rVB2	692	550	0.02%	0.003%
29	6.809	1792	1794	1797	rBV2	261	194	0.01%	0.001%
30	6.860	1808	1810	1813	rVB	574	230	0.01%	0.001%
31	6.905	1813	1824	1856	rBV	287235	561501	22.08%	2.928%
32	7.233	1916	1926	1955	rBV	1116165	1986007	78.10%	10.356%
33	7.548	2015	2024	2052	rBV	195111	362841	14.27%	1.892%
34	7.854	2116	2119	2121	rBV	1077	662	0.03%	0.003%
35	7.950	2144	2149	2153	rBV6	790	911	0.04%	0.005%
36	8.024	2163	2172	2220	rBV2	325870	729384	28.68%	3.803%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037851.D
 Acq On : 14 Oct 2024 13:08
 Operator : SY/MD
 Sample : P4379-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.545	2329	2334	2336	rBV5	2461	2480	0.10%	0.013%
38	8.648	2364	2366	2369	rBV2	672	502	0.02%	0.003%
39	8.776	2394	2406	2446	rBV	1347822	2215102	87.11%	11.550%
40	9.297	2565	2568	2571	rBV3	915	716	0.03%	0.004%
41	9.336	2578	2580	2582	rVB	426	112	0.00%	0.001%
42	9.349	2582	2584	2587	rBV2	568	311	0.01%	0.002%
43	9.368	2587	2590	2596	rVB6	1014	784	0.03%	0.004%
44	9.394	2596	2598	2599	rBV2	826	346	0.01%	0.002%
45	9.426	2605	2608	2617	rBV5	714	1116	0.04%	0.006%
46	9.465	2617	2620	2621	rBV2	348	197	0.01%	0.001%
47	9.471	2621	2622	2624	rBV2	403	137	0.01%	0.001%
48	9.484	2624	2626	2629	rBV4	634	444	0.02%	0.002%
49	9.555	2646	2648	2650	rBV2	555	282	0.01%	0.001%
50	9.603	2660	2663	2666	rBV4	758	548	0.02%	0.003%
51	9.616	2666	2667	2672	rVB3	900	479	0.02%	0.002%
52	9.699	2690	2693	2695	rBV3	839	483	0.02%	0.003%
53	9.725	2699	2701	2702	rVV	232	65	0.00%	0.000%
54	9.744	2703	2707	2710	rVV2	654	570	0.02%	0.003%
55	9.764	2710	2713	2716	rVV4	669	548	0.02%	0.003%
56	9.796	2720	2723	2726	rBV2	507	384	0.02%	0.002%
57	9.831	2731	2734	2736	rBV	794	442	0.02%	0.002%
58	9.844	2736	2738	2740	rBV2	418	182	0.01%	0.001%
59	9.857	2740	2742	2744	rBV2	435	137	0.01%	0.001%
60	9.940	2761	2768	2774	rBV5	1095	1792	0.07%	0.009%
61	10.002	2785	2787	2791	rBV3	224	103	0.00%	0.001%
62	10.030	2795	2796	2798	rVB	428	95	0.00%	0.000%
63	10.053	2802	2803	2805	rBV	282	128	0.01%	0.001%
64	10.101	2814	2818	2820	rVB2	826	559	0.02%	0.003%
65	10.146	2820	2832	2856	rBV	657034	1042931	41.02%	5.438%
66	10.468	2929	2932	2934	rBV2	617	417	0.02%	0.002%
67	10.567	2961	2963	2965	rVB2	315	102	0.00%	0.001%
68	10.577	2965	2966	2968	rBV2	714	346	0.01%	0.002%
69	10.616	2974	2978	2980	rBV3	970	717	0.03%	0.004%
70	10.648	2986	2988	2990	rBV	415	170	0.01%	0.001%
71	10.731	3011	3014	3015	rBV4	616	335	0.01%	0.002%
72	10.767	3023	3025	3026	rBV	411	137	0.01%	0.001%
73	10.783	3026	3030	3033	rVV2	1132	998	0.04%	0.005%
74	10.915	3069	3071	3073	rBV	437	194	0.01%	0.001%
75	10.966	3083	3087	3090	rBV3	835	548	0.02%	0.003%
76	10.998	3094	3097	3103	rVB5	1047	617	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037851.D
 Acq On : 14 Oct 2024 13:08
 Operator : SY/MD
 Sample : P4379-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

77	11.027	3103	3106	3107	rBV2	267	188	0.01%	0.001%
78	11.037	3107	3109	3115	rVB4	772	482	0.02%	0.003%
79	11.178	3142	3153	3187	rBV	1294715	2062532	81.11%	10.755%
80	11.551	3258	3269	3299	rBV	1179019	1882462	74.03%	9.816%
81	12.593	3591	3593	3597	rBV4	1124	828	0.03%	0.004%
82	13.011	3721	3723	3726	rBV2	743	422	0.02%	0.002%
83	13.407	3844	3846	3850	rVB2	1124	619	0.02%	0.003%
84	13.612	3905	3910	3912	rBV4	1021	949	0.04%	0.005%
85	13.661	3923	3925	3930	rBV3	925	682	0.03%	0.004%




Sum of corrected areas: 19177712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037851.D
Acq On : 14 Oct 2024 13:08
Operator : SY/MD
Sample : P4379-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

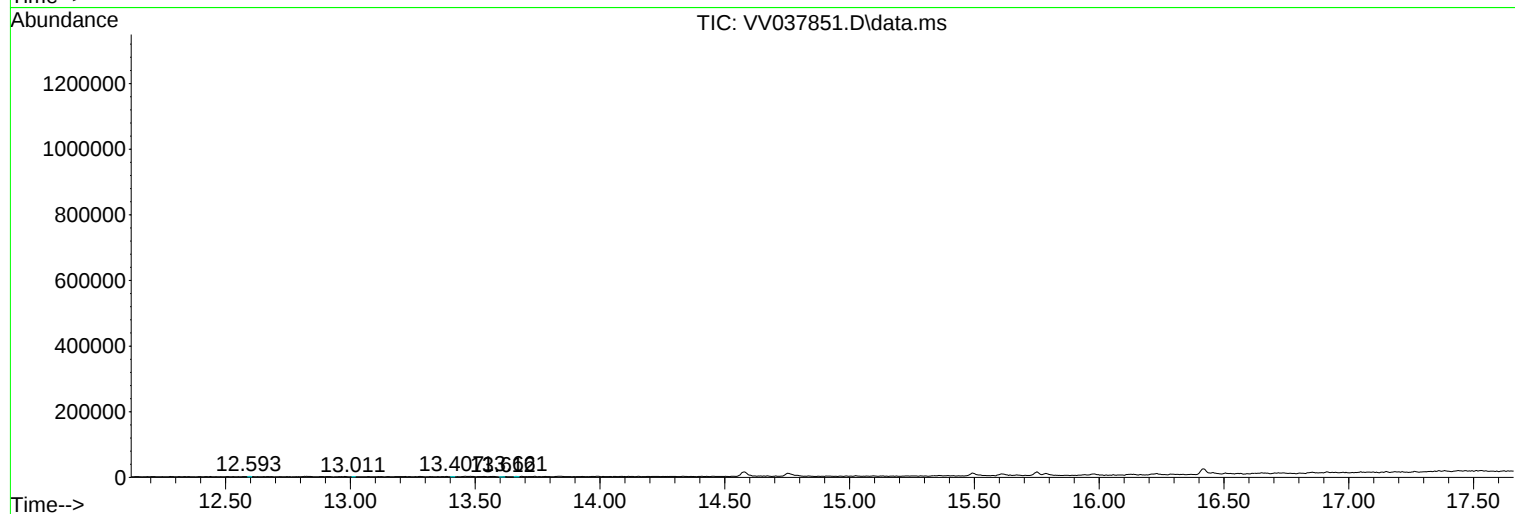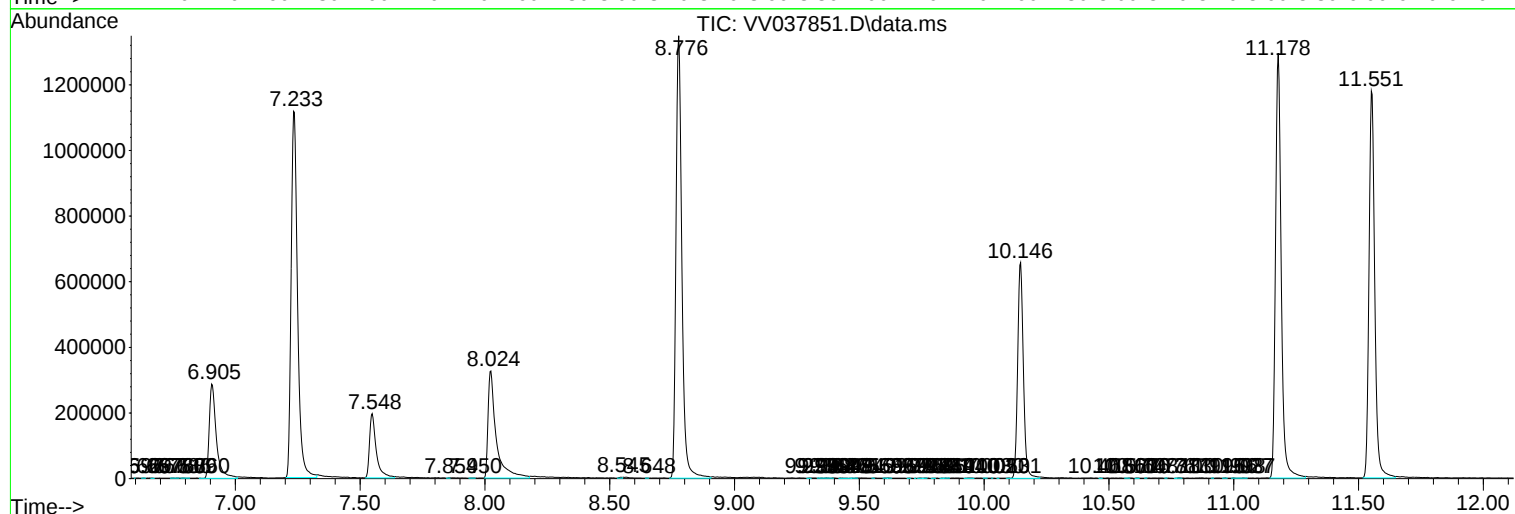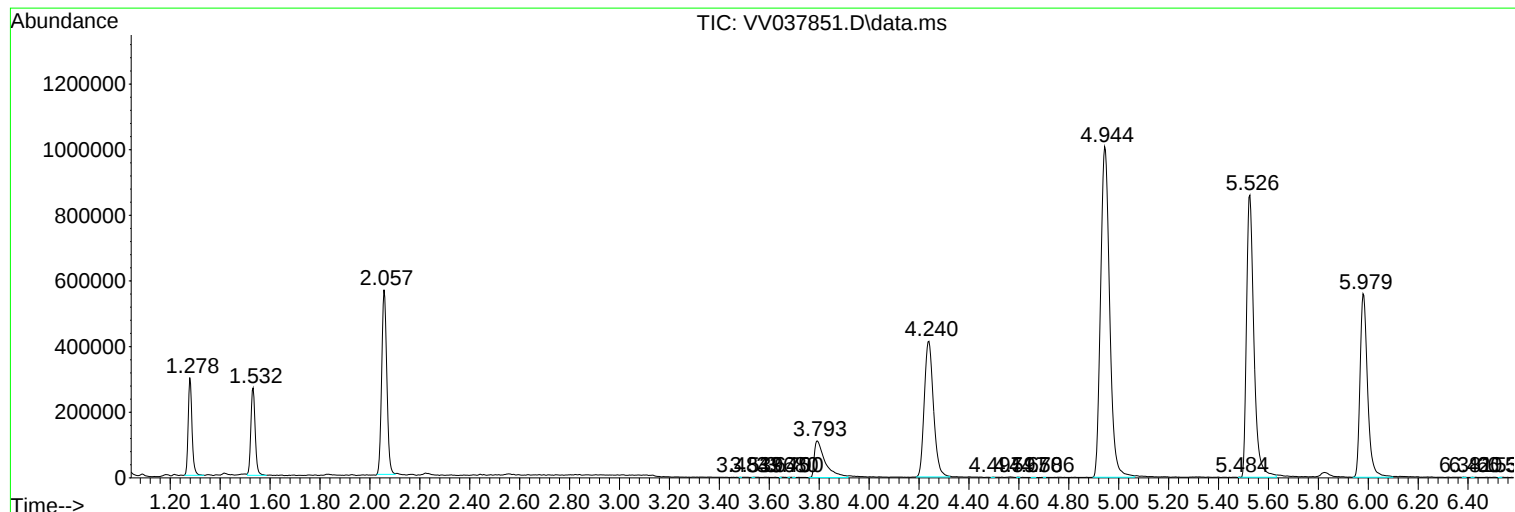

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037851.D
Acq On : 14 Oct 2024 13:08
Operator : SY/MD
Sample : P4379-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037851.D
Acq On : 14 Oct 2024 13:08
Operator : SY/MD
Sample : P4379-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------