

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037852.D
 Acq On : 14 Oct 2024 13:29
 Operator : SY/MD
 Sample : P4379-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.089	10	15	26	rVB2	11769	13664	0.59%	0.080%
2	1.188	37	46	52	rBV3	7327	13856	0.60%	0.081%
3	1.217	52	55	61	rVV	3561	4101	0.18%	0.024%
4	1.278	67	74	88	rBV	262597	277842	11.97%	1.633%
5	1.532	145	153	168	rVB	245003	289063	12.45%	1.699%
6	2.060	307	317	331	rBV	509647	725490	31.25%	4.264%
7	3.439	741	746	750	rBV4	696	575	0.02%	0.003%
8	3.587	788	792	795	rVB2	782	574	0.02%	0.003%
9	3.606	795	798	800	rBV2	604	508	0.02%	0.003%
10	3.651	810	812	817	rVB3	828	617	0.03%	0.004%
11	3.799	849	858	889	rBV	103540	306591	13.21%	1.802%
12	4.101	949	952	959	rVB4	920	1114	0.05%	0.007%
13	4.153	965	968	970	rBV2	985	644	0.03%	0.004%
14	4.243	979	996	1027	rBV	384782	972929	41.91%	5.718%
15	4.532	1084	1086	1091	rVB4	855	621	0.03%	0.004%
16	4.558	1091	1094	1096	rBV2	853	555	0.02%	0.003%
17	4.896	1189	1199	1201	rBV3	1012	1386	0.06%	0.008%
18	4.947	1201	1215	1250	rBV2	910547	2321226	100.00%	13.641%
19	5.281	1316	1319	1321	rVV3	702	514	0.02%	0.003%
20	5.317	1325	1330	1336	rVB7	1480	1578	0.07%	0.009%
21	5.413	1357	1360	1361	rBV3	870	552	0.02%	0.003%
22	5.461	1372	1375	1380	rVB4	656	505	0.02%	0.003%
23	5.529	1385	1396	1431	rBV	687094	1418801	61.12%	8.338%
24	5.834	1480	1491	1503	rBV5	10422	24074	1.04%	0.141%
25	5.982	1524	1537	1571	rVV	514391	1080541	46.55%	6.350%
26	6.252	1618	1621	1625	rBV4	705	532	0.02%	0.003%
27	6.272	1625	1627	1630	rVB3	959	603	0.03%	0.004%
28	6.317	1637	1641	1646	rVB2	791	811	0.03%	0.005%
29	6.381	1656	1661	1663	rBV3	1063	917	0.04%	0.005%
30	6.397	1663	1666	1670	rVB3	796	631	0.03%	0.004%
31	6.426	1670	1675	1678	rVB5	1170	779	0.03%	0.005%
32	6.477	1688	1691	1696	rVB4	700	577	0.02%	0.003%
33	6.506	1696	1700	1702	rBV2	613	550	0.02%	0.003%
34	6.658	1740	1747	1749	rBV7	539	583	0.03%	0.003%
35	6.744	1769	1774	1775	rBV2	1260	803	0.03%	0.005%
36	6.786	1784	1787	1791	rVB4	999	798	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037852.D
 Acq On : 14 Oct 2024 13:29
 Operator : SY/MD
 Sample : P4379-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.908	1810	1825	1848	rBV	256428	499606	21.52%	2.936%
38	7.111	1887	1888	1895	rVB5	764	572	0.02%	0.003%
39	7.198	1909	1915	1916	rBV4	1170	1011	0.04%	0.006%
40	7.236	1916	1927	1958	rBV	1038562	1829361	78.81%	10.751%
41	7.548	2015	2024	2044	rBV	173548	322350	13.89%	1.894%
42	7.973	2150	2156	2158	rBV4	950	899	0.04%	0.005%
43	8.024	2164	2172	2215	rBV2	307111	687306	29.61%	4.039%
44	8.394	2285	2287	2297	rVB7	1110	1484	0.06%	0.009%
45	8.548	2332	2335	2338	rVV5	1302	1115	0.05%	0.007%
46	8.776	2395	2406	2447	rVV	1067766	1807001	77.85%	10.619%
47	9.146	2518	2521	2523	rVB3	1243	792	0.03%	0.005%
48	9.204	2535	2539	2541	rVB5	852	627	0.03%	0.004%
49	9.230	2541	2547	2552	rBV4	678	765	0.03%	0.004%
50	9.342	2580	2582	2587	rVB4	853	719	0.03%	0.004%
51	9.413	2598	2604	2609	rBV5	764	874	0.04%	0.005%
52	9.522	2636	2638	2644	rVB3	969	739	0.03%	0.004%
53	9.773	2711	2716	2720	rVB4	848	883	0.04%	0.005%
54	9.809	2723	2727	2733	rVB5	911	997	0.04%	0.006%
55	9.876	2744	2748	2751	rBV3	813	604	0.03%	0.004%
56	10.001	2781	2787	2790	rBV3	782	841	0.04%	0.005%
57	10.034	2790	2797	2800	rBV4	621	576	0.02%	0.003%
58	10.053	2800	2803	2808	rVB4	730	633	0.03%	0.004%
59	10.146	2817	2832	2855	rBV	613726	980242	42.23%	5.761%
60	10.834	3041	3046	3048	rBV2	699	553	0.02%	0.003%
61	10.863	3048	3055	3058	rVV6	859	971	0.04%	0.006%
62	10.976	3088	3090	3096	rBV2	566	574	0.02%	0.003%
63	11.037	3105	3109	3111	rBV3	689	528	0.02%	0.003%
64	11.127	3132	3137	3139	rBV3	1082	926	0.04%	0.005%
65	11.178	3142	3153	3185	rBV	1033985	1649845	71.08%	9.696%
66	11.464	3237	3242	3249	rVB7	1480	1533	0.07%	0.009%
67	11.493	3249	3251	3255	rBV3	731	601	0.03%	0.004%
68	11.554	3257	3270	3298	rBV	1055615	1725778	74.35%	10.142%
69	11.982	3401	3403	3408	rVB4	1059	664	0.03%	0.004%
70	12.021	3411	3415	3418	rBV3	689	491	0.02%	0.003%
71	12.085	3429	3435	3437	rBV4	1269	1005	0.04%	0.006%
72	12.098	3437	3439	3443	rVV4	1067	602	0.03%	0.004%
73	12.133	3447	3450	3455	rVV4	846	790	0.03%	0.005%
74	12.300	3498	3502	3506	rVV4	775	538	0.02%	0.003%
75	12.329	3509	3511	3515	rBV4	737	490	0.02%	0.003%
76	12.384	3524	3528	3535	rVB4	816	916	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037852.D
 Acq On : 14 Oct 2024 13:29
 Operator : SY/MD
 Sample : P4379-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.448	3545	3548	3551	rBV2	729	559	0.02%	0.003%
78	12.497	3560	3563	3568	rBV4	1251	984	0.04%	0.006%
79	12.615	3598	3600	3603	rBV2	1115	688	0.03%	0.004%
80	12.718	3629	3632	3635	rBV4	1042	719	0.03%	0.004%
81	12.792	3653	3655	3658	rBV4	801	562	0.02%	0.003%
82	12.873	3678	3680	3687	rVB5	907	972	0.04%	0.006%
83	12.953	3701	3705	3708	rBV3	963	724	0.03%	0.004%
84	13.033	3728	3730	3737	rVB2	1059	815	0.04%	0.005%
85	13.091	3742	3748	3750	rBV5	848	921	0.04%	0.005%
86	13.169	3770	3772	3775	rBV4	772	507	0.02%	0.003%
87	13.397	3840	3843	3846	rBV2	779	651	0.03%	0.004%
88	13.648	3918	3921	3927	rVB2	840	810	0.03%	0.005%
89	13.744	3947	3951	3953	rBV3	911	523	0.02%	0.003%
90	13.770	3956	3959	3962	rBV2	730	544	0.02%	0.003%
91	13.841	3978	3981	3986	rBV4	649	519	0.02%	0.003%
92	14.046	4043	4045	4048	rBV3	825	491	0.02%	0.003%
93	14.426	4159	4163	4164	rBV3	813	600	0.03%	0.004%
94	14.516	4188	4191	4194	rBV4	855	522	0.02%	0.003%
95	14.580	4206	4211	4215	rBV4	3728	4280	0.18%	0.025%
96	14.853	4292	4296	4298	rBV4	1248	1031	0.04%	0.006%
97	14.892	4306	4308	4311	rBV4	907	597	0.03%	0.004%
98	15.072	4361	4364	4366	rBV3	853	598	0.03%	0.004%
99	15.242	4415	4417	4420	rVB2	1073	529	0.02%	0.003%
100	15.496	4490	4496	4502	rBV8	2807	4724	0.20%	0.028%




Sum of corrected areas: 17016177

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037852.D
Acq On : 14 Oct 2024 13:29
Operator : SY/MD
Sample : P4379-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

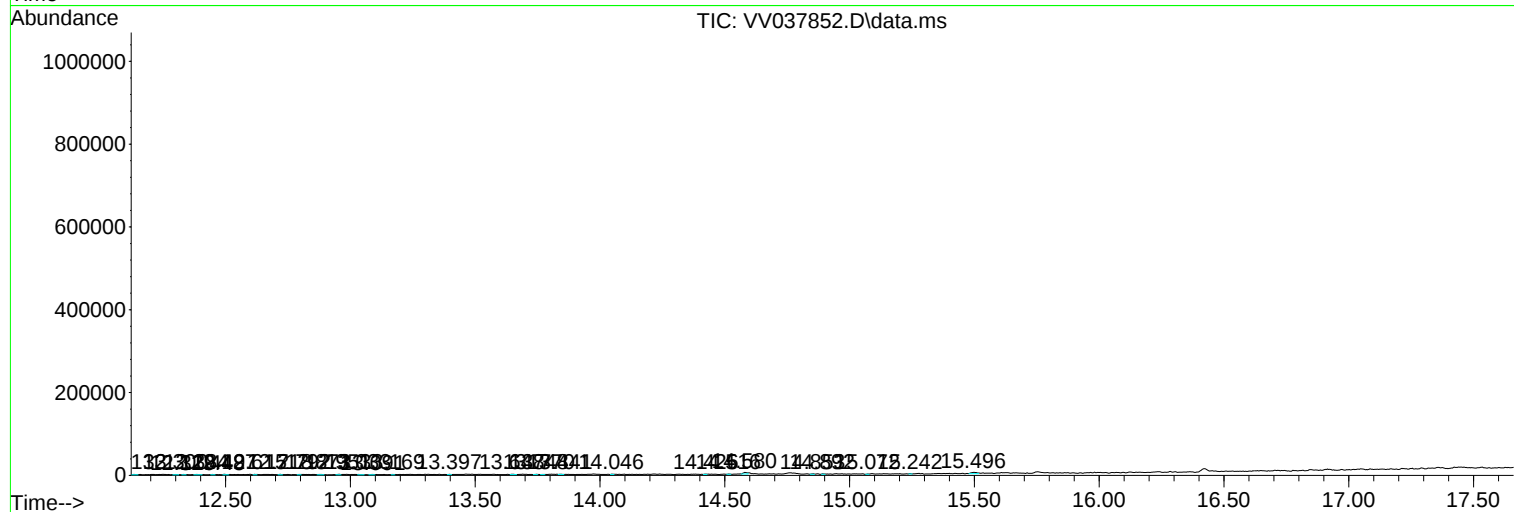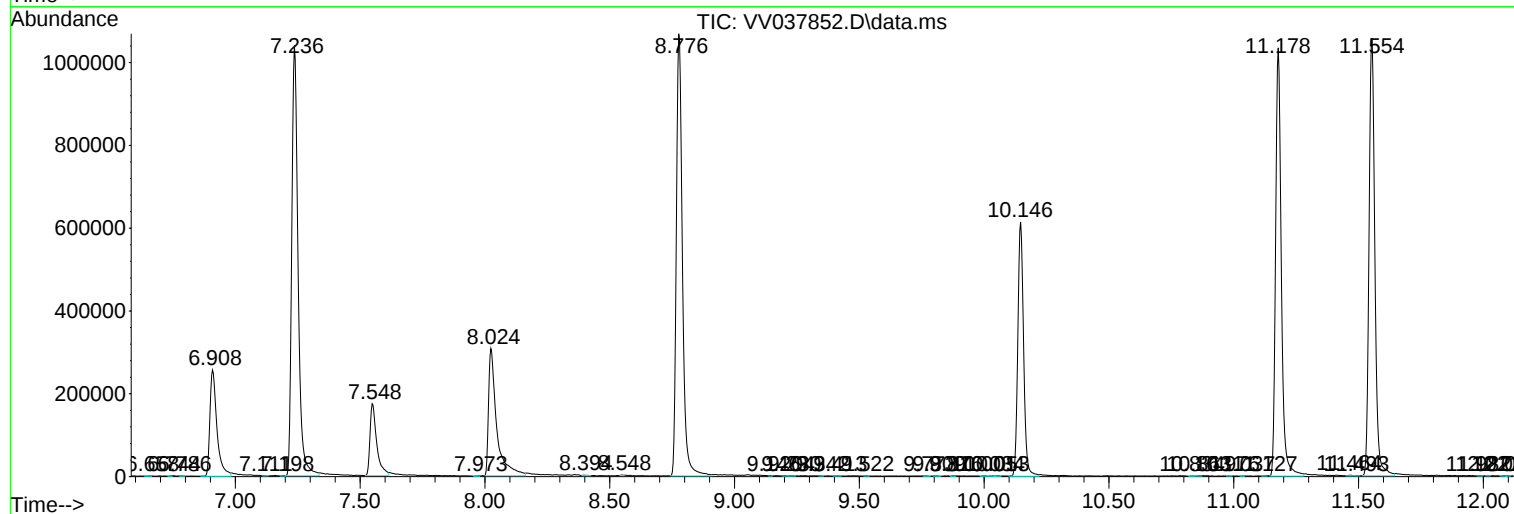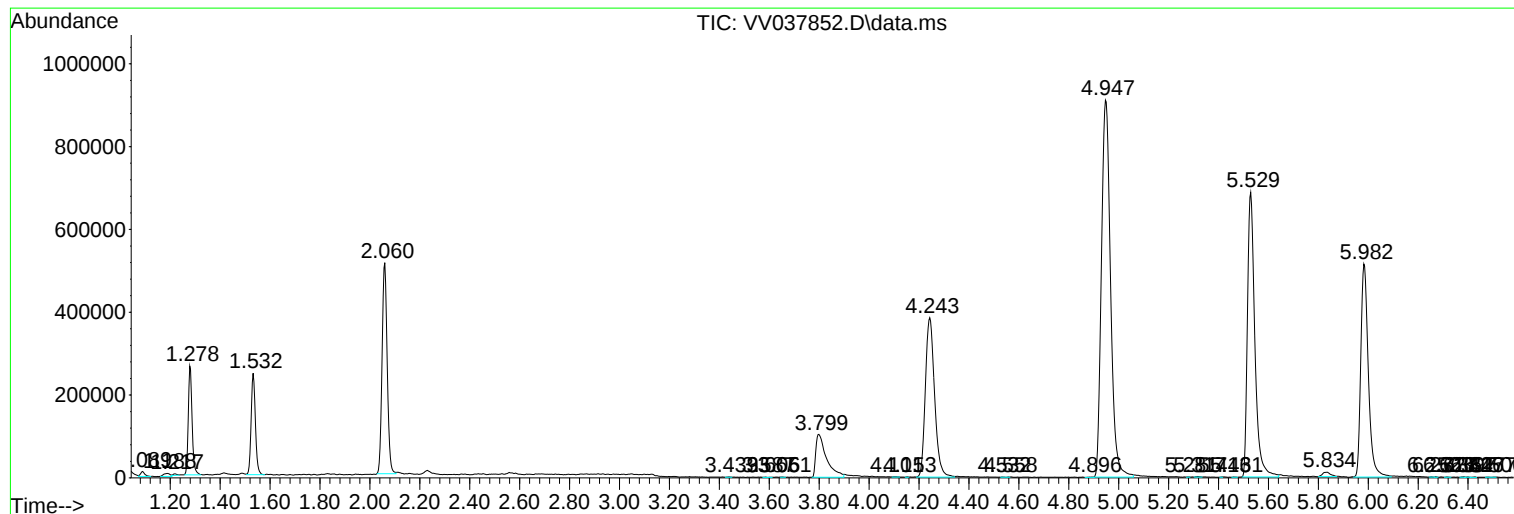

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037852.D
Acq On : 14 Oct 2024 13:29
Operator : SY/MD
Sample : P4379-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037852.D
Acq On : 14 Oct 2024 13:29
Operator : SY/MD
Sample : P4379-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------