

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037853.D
 Acq On : 14 Oct 2024 13:51
 Operator : SY/MD
 Sample : P4379-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB	257377	275698	12.25%	1.662%
2	1.532	146	153	166	rVB	243500	276312	12.28%	1.666%
3	2.060	308	317	332	rBV	487232	695059	30.89%	4.190%
4	3.343	713	716	718	rBV4	353	237	0.01%	0.001%
5	3.465	750	754	757	rBV2	766	542	0.02%	0.003%
6	3.535	772	776	781	rBV5	826	848	0.04%	0.005%
7	3.564	783	785	788	rVB2	793	384	0.02%	0.002%
8	3.580	788	790	793	rBV2	369	233	0.01%	0.001%
9	3.622	799	803	806	rBV2	599	628	0.03%	0.004%
10	3.725	834	835	837	rBV	384	193	0.01%	0.001%
11	3.799	849	858	893	rBV	101925	310566	13.80%	1.872%
12	4.243	981	996	1029	rVB	367245	929397	41.31%	5.603%
13	4.580	1098	1101	1104	rBV2	799	517	0.02%	0.003%
14	4.629	1114	1116	1119	rVB4	535	328	0.01%	0.002%
15	4.654	1119	1124	1127	rBV5	723	622	0.03%	0.004%
16	4.674	1128	1130	1134	rVB	527	271	0.01%	0.002%
17	4.699	1134	1138	1141	rVB3	575	446	0.02%	0.003%
18	4.719	1141	1144	1145	rBV	439	196	0.01%	0.001%
19	4.728	1145	1147	1149	rBV2	544	331	0.01%	0.002%
20	4.828	1175	1178	1181	rBV2	413	277	0.01%	0.002%
21	4.879	1192	1194	1197	rVB2	694	346	0.02%	0.002%
22	4.896	1197	1199	1200	rBV2	481	248	0.01%	0.001%
23	4.947	1200	1215	1252	rBV2	883896	2249807	100.00%	13.564%
24	5.391	1351	1353	1356	rBV2	750	373	0.02%	0.002%
25	5.471	1376	1378	1380	rBV2	367	189	0.01%	0.001%
26	5.529	1385	1396	1424	rBV	697032	1435666	63.81%	8.656%
27	5.828	1481	1489	1504	rVB3	11924	26486	1.18%	0.160%
28	5.982	1525	1537	1568	rBV	499244	1043049	46.36%	6.288%
29	6.297	1634	1635	1638	rVB3	822	300	0.01%	0.002%
30	6.365	1654	1656	1660	rVB3	1233	676	0.03%	0.004%
31	6.522	1703	1705	1706	rBV	627	232	0.01%	0.001%
32	6.561	1715	1717	1720	rBV	397	260	0.01%	0.002%
33	6.603	1728	1730	1732	rBV	618	258	0.01%	0.002%
34	6.635	1737	1740	1742	rVV2	633	401	0.02%	0.002%
35	6.648	1742	1744	1747	rVV4	378	311	0.01%	0.002%
36	6.670	1750	1751	1755	rVB3	649	307	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037853.D
 Acq On : 14 Oct 2024 13:51
 Operator : SY/MD
 Sample : P4379-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.709	1760	1763	1766	rBV3	560	418	0.02%	0.003%
38	6.760	1773	1779	1782	rBV4	763	808	0.04%	0.005%
39	6.805	1788	1793	1795	rVB3	688	410	0.02%	0.002%
40	6.825	1795	1799	1801	rBV4	446	355	0.02%	0.002%
41	6.908	1815	1825	1857	rBV	251672	488769	21.72%	2.947%
42	7.162	1903	1904	1906	rBV2	643	314	0.01%	0.002%
43	7.236	1916	1927	1962	rBV	993746	1770442	78.69%	10.674%
44	7.506	2008	2011	2015	rBV5	1008	756	0.03%	0.005%
45	7.551	2016	2025	2057	rVV	169464	320083	14.23%	1.930%
46	7.963	2152	2153	2155	rBV	564	185	0.01%	0.001%
47	8.024	2164	2172	2206	rBV2	303334	654657	29.10%	3.947%
48	8.696	2378	2381	2389	rVB6	764	596	0.03%	0.004%
49	8.776	2395	2406	2440	rBV	1082307	1813356	80.60%	10.933%
50	9.223	2543	2545	2549	rBV3	932	696	0.03%	0.004%
51	9.272	2553	2560	2565	rBV5	830	1148	0.05%	0.007%
52	9.326	2574	2577	2581	rBV2	953	678	0.03%	0.004%
53	9.362	2584	2588	2592	rBV4	630	620	0.03%	0.004%
54	9.410	2600	2603	2604	rBV2	563	327	0.01%	0.002%
55	9.551	2644	2647	2649	rBV2	485	296	0.01%	0.002%
56	9.606	2662	2664	2667	rBV	596	315	0.01%	0.002%
57	9.641	2672	2675	2679	rBV2	512	372	0.02%	0.002%
58	9.699	2689	2693	2696	rVV	815	533	0.02%	0.003%
59	9.719	2696	2699	2703	rBV3	395	385	0.02%	0.002%
60	9.751	2707	2709	2713	rBV3	763	514	0.02%	0.003%
61	9.770	2713	2715	2716	rBV	440	165	0.01%	0.001%
62	9.815	2726	2729	2731	rBV	561	396	0.02%	0.002%
63	9.844	2736	2738	2741	rBV	460	212	0.01%	0.001%
64	9.863	2741	2744	2746	rBV2	713	537	0.02%	0.003%
65	9.915	2758	2760	2763	rVB2	307	171	0.01%	0.001%
66	9.966	2774	2776	2780	rVB2	598	309	0.01%	0.002%
67	9.995	2782	2785	2788	rBV2	989	727	0.03%	0.004%
68	10.014	2788	2791	2792	rBV2	589	299	0.01%	0.002%
69	10.043	2798	2800	2801	rBV	418	164	0.01%	0.001%
70	10.088	2812	2814	2816	rBV2	420	197	0.01%	0.001%
71	10.146	2821	2832	2864	rVV	591481	947384	42.11%	5.712%
72	10.574	2962	2965	2967	rVB3	499	293	0.01%	0.002%
73	10.596	2970	2972	2976	rVB2	580	311	0.01%	0.002%
74	10.625	2976	2981	2984	rBV4	418	407	0.02%	0.002%
75	10.641	2984	2986	2992	rBV3	411	401	0.02%	0.002%
76	10.673	2993	2996	2999	rVB3	537	327	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037853.D
 Acq On : 14 Oct 2024 13:51
 Operator : SY/MD
 Sample : P4379-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.693	2999	3002	3004	rBV2	766	434	0.02%	0.003%
78	10.725	3009	3012	3018	rBV4	614	660	0.03%	0.004%
79	10.747	3018	3019	3024	rVB3	647	365	0.02%	0.002%
80	10.783	3024	3030	3034	rBV6	1469	1862	0.08%	0.011%
81	10.863	3049	3055	3059	rVB4	956	1145	0.05%	0.007%
82	10.889	3061	3063	3066	rVV	405	167	0.01%	0.001%
83	10.944	3076	3080	3085	rBV3	474	551	0.02%	0.003%
84	10.982	3090	3092	3094	rVV2	606	312	0.01%	0.002%
85	10.995	3094	3096	3099	rVV	599	391	0.02%	0.002%
86	11.021	3103	3104	3107	rVV2	465	241	0.01%	0.001%
87	11.050	3111	3113	3119	rVB2	416	350	0.02%	0.002%
88	11.178	3142	3153	3189	rBV	1022321	1653459	73.49%	9.969%
89	11.551	3258	3269	3297	rBV	1027219	1658823	73.73%	10.001%
90	12.027	3415	3417	3420	rBV3	433	211	0.01%	0.001%
91	12.043	3420	3422	3426	rBV2	785	534	0.02%	0.003%
92	12.114	3442	3444	3449	rVB5	736	549	0.02%	0.003%
93	12.207	3469	3473	3477	rBV5	1211	965	0.04%	0.006%
94	12.281	3495	3496	3498	rBV	406	201	0.01%	0.001%
95	12.355	3516	3519	3522	rBV3	867	665	0.03%	0.004%
96	12.577	3586	3588	3592	rBV3	807	572	0.03%	0.003%
97	12.686	3620	3622	3629	rBV5	853	659	0.03%	0.004%
98	12.850	3670	3673	3677	rBV3	745	788	0.04%	0.005%
99	13.091	3744	3748	3751	rBV3	1038	845	0.04%	0.005%
100	13.349	3825	3828	3829	rBV2	1126	594	0.03%	0.004%




Sum of corrected areas: 16586670

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037853.D
Acq On : 14 Oct 2024 13:51
Operator : SY/MD
Sample : P4379-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

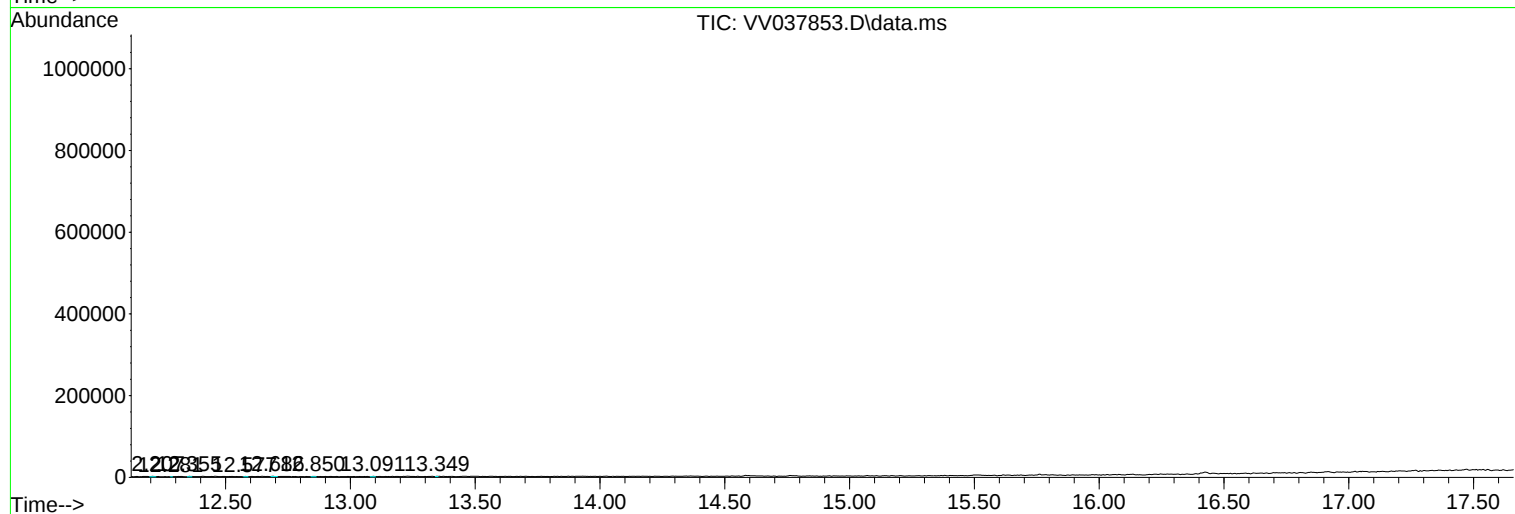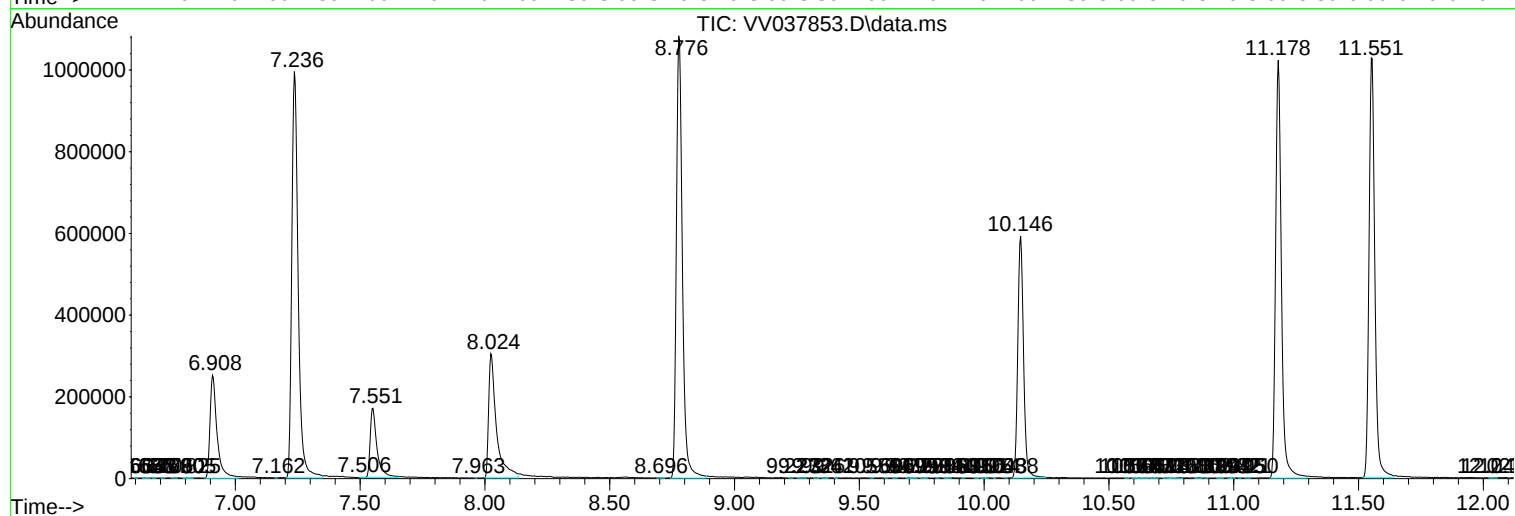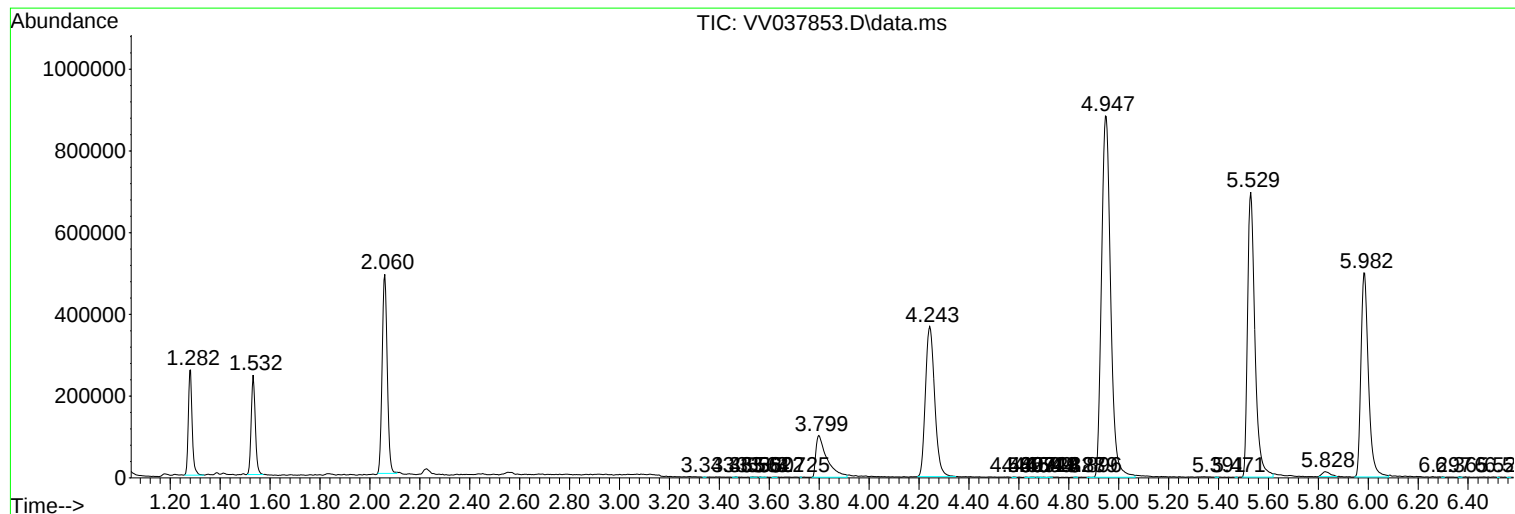

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037853.D
Acq On : 14 Oct 2024 13:51
Operator : SY/MD
Sample : P4379-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037853.D
Acq On : 14 Oct 2024 13:51
Operator : SY/MD
Sample : P4379-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------