

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037856.D
 Acq On : 14 Oct 2024 15:00
 Operator : SY/MD
 Sample : P4379-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	35	42	50	rBV3	4489	7818	0.34%	0.046%
2	1.220	52	56	66	rVV3	4980	6978	0.30%	0.041%
3	1.278	67	74	89	rVV	257790	280545	12.10%	1.643%
4	1.532	145	153	168	rVB	250867	293933	12.68%	1.721%
5	2.056	306	316	332	rBV	505495	733575	31.64%	4.295%
6	3.407	733	736	738	rBV3	652	502	0.02%	0.003%
7	3.625	801	804	807	rVB3	730	486	0.02%	0.003%
8	3.796	849	857	891	rBV	98916	289891	12.51%	1.697%
9	4.239	975	995	1030	rBV	383205	979145	42.24%	5.733%
10	4.468	1064	1066	1070	rVB2	854	488	0.02%	0.003%
11	4.741	1147	1151	1154	rBV3	872	559	0.02%	0.003%
12	4.866	1186	1190	1193	rBV2	1080	962	0.04%	0.006%
13	4.947	1199	1215	1245	rBV2	923667	2318164	100.00%	13.573%
14	5.217	1292	1299	1300	rBV5	916	965	0.04%	0.006%
15	5.243	1304	1307	1311	rVB4	868	598	0.03%	0.004%
16	5.268	1311	1315	1316	rBV3	905	689	0.03%	0.004%
17	5.526	1384	1395	1436	rVV	704616	1475983	63.67%	8.642%
18	5.825	1479	1488	1509	rVB3	14341	36100	1.56%	0.211%
19	5.982	1524	1537	1565	rBV	517875	1064821	45.93%	6.235%
20	6.243	1615	1618	1623	rVB3	1155	885	0.04%	0.005%
21	6.300	1632	1636	1639	rVB4	1013	830	0.04%	0.005%
22	6.509	1696	1701	1704	rVB4	585	477	0.02%	0.003%
23	6.554	1711	1715	1718	rVB4	817	629	0.03%	0.004%
24	6.580	1718	1723	1727	rVB4	606	610	0.03%	0.004%
25	6.799	1785	1791	1794	rVV4	731	735	0.03%	0.004%
26	6.908	1815	1825	1854	rBV	252644	500938	21.61%	2.933%
27	7.117	1888	1890	1896	rVB5	1019	958	0.04%	0.006%
28	7.175	1904	1908	1912	rBV6	1048	962	0.04%	0.006%
29	7.236	1914	1927	1955	rBV	1023432	1808152	78.00%	10.587%
30	7.513	2011	2013	2015	rBV3	1176	655	0.03%	0.004%
31	7.548	2015	2024	2053	rVV	170247	330493	14.26%	1.935%
32	7.850	2115	2118	2121	rBV4	915	729	0.03%	0.004%
33	7.866	2121	2123	2129	rVB6	899	574	0.02%	0.003%
34	7.934	2142	2144	2149	rVB4	1005	847	0.04%	0.005%
35	7.960	2149	2152	2159	rVB3	547	619	0.03%	0.004%
36	8.024	2164	2172	2206	rBV2	299766	662193	28.57%	3.877%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037856.D
 Acq On : 14 Oct 2024 15:00
 Operator : SY/MD
 Sample : P4379-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.458	2303	2307	2310	rBV3	771	713	0.03%	0.004%
38	8.522	2324	2327	2329	rBV3	652	491	0.02%	0.003%
39	8.554	2333	2337	2340	rVV6	1918	1987	0.09%	0.012%
40	8.705	2380	2384	2387	rBV4	850	619	0.03%	0.004%
41	8.776	2395	2406	2442	rBV	1128992	1869775	80.66%	10.948%
42	9.050	2486	2491	2492	rBV4	1280	1186	0.05%	0.007%
43	9.162	2523	2526	2529	rVB3	1340	958	0.04%	0.006%
44	9.197	2529	2537	2538	rBV3	618	771	0.03%	0.005%
45	9.275	2557	2561	2564	rBV3	1172	861	0.04%	0.005%
46	9.294	2564	2567	2571	rVB4	838	621	0.03%	0.004%
47	9.390	2592	2597	2600	rBV4	721	822	0.04%	0.005%
48	9.625	2665	2670	2673	rBV2	587	651	0.03%	0.004%
49	9.805	2720	2726	2731	rVB5	780	808	0.03%	0.005%
50	10.011	2784	2790	2794	rVB5	572	560	0.02%	0.003%
51	10.146	2817	2832	2852	rBV	600923	968649	41.79%	5.672%
52	10.313	2881	2884	2890	rVB4	1227	1033	0.04%	0.006%
53	10.455	2923	2928	2931	rVB2	781	539	0.02%	0.003%
54	10.474	2931	2934	2936	rBV2	877	566	0.02%	0.003%
55	10.516	2944	2947	2949	rVB	865	527	0.02%	0.003%
56	10.535	2949	2953	2957	rBV3	985	888	0.04%	0.005%
57	10.606	2973	2975	2980	rVV3	586	498	0.02%	0.003%
58	10.641	2980	2986	2992	rVB5	1015	1158	0.05%	0.007%
59	10.676	2992	2997	3000	rBV5	799	641	0.03%	0.004%
60	10.741	3012	3017	3022	rBV3	888	1292	0.06%	0.008%
61	11.178	3142	3153	3179	rBV	1059350	1682016	72.56%	9.848%
62	11.554	3257	3270	3298	rBV	1059414	1709652	73.75%	10.010%
63	11.811	3348	3350	3354	rBV4	984	603	0.03%	0.004%
64	11.943	3388	3391	3395	rBV5	819	671	0.03%	0.004%
65	12.014	3410	3413	3417	rBV4	690	720	0.03%	0.004%
66	12.065	3426	3429	3431	rVB3	923	538	0.02%	0.003%
67	12.085	3431	3435	3439	rVV5	833	729	0.03%	0.004%
68	12.136	3449	3451	3455	rVV2	731	521	0.02%	0.003%
69	12.159	3455	3458	3461	rVV2	823	678	0.03%	0.004%
70	12.191	3465	3468	3471	rVV3	1154	904	0.04%	0.005%
71	12.217	3473	3476	3479	rVV3	1146	827	0.04%	0.005%
72	12.246	3482	3485	3489	rVV2	671	631	0.03%	0.004%
73	12.316	3501	3507	3508	rBV3	917	798	0.03%	0.005%
74	12.329	3508	3511	3514	rBV4	696	495	0.02%	0.003%
75	12.464	3551	3553	3557	rVB3	696	491	0.02%	0.003%
76	12.490	3557	3561	3564	rBV2	645	499	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037856.D
 Acq On : 14 Oct 2024 15:00
 Operator : SY/MD
 Sample : P4379-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.609	3596	3598	3605	rVB4	661	633	0.03%	0.004%
78	12.702	3625	3627	3630	rBV3	813	482	0.02%	0.003%
79	12.721	3631	3633	3638	rVB3	975	652	0.03%	0.004%
80	12.763	3642	3646	3648	rBV2	604	491	0.02%	0.003%
81	12.779	3649	3651	3655	rVB3	906	766	0.03%	0.004%
82	12.950	3697	3704	3712	rBV4	918	1773	0.08%	0.010%
83	13.078	3740	3744	3747	rVB2	957	671	0.03%	0.004%
84	13.226	3787	3790	3793	rBV3	699	570	0.02%	0.003%
85	13.332	3819	3823	3827	rBV4	850	1010	0.04%	0.006%
86	13.387	3836	3840	3842	rBV2	936	749	0.03%	0.004%
87	13.503	3872	3876	3880	rBV4	1108	845	0.04%	0.005%
88	13.590	3900	3903	3905	rBV3	887	482	0.02%	0.003%
89	13.709	3938	3940	3944	rVB4	1124	628	0.03%	0.004%
90	13.741	3944	3950	3952	rBV4	982	1005	0.04%	0.006%
91	13.876	3988	3992	3994	rBV3	705	574	0.02%	0.003%
92	13.979	4019	4024	4026	rBV3	1045	880	0.04%	0.005%
93	14.014	4033	4035	4041	rVB4	873	638	0.03%	0.004%
94	14.104	4058	4063	4066	rBV4	775	744	0.03%	0.004%
95	14.474	4174	4178	4179	rBV2	1061	665	0.03%	0.004%
96	14.721	4252	4255	4259	rBV2	824	604	0.03%	0.004%
97	14.763	4266	4268	4273	rVB5	1224	1032	0.04%	0.006%
98	14.905	4310	4312	4315	rBV3	883	523	0.02%	0.003%
99	15.178	4393	4397	4400	rBV4	1590	1219	0.05%	0.007%
100	15.667	4547	4549	4552	rBV3	1301	722	0.03%	0.004%




Sum of corrected areas: 17079233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037856.D
Acq On : 14 Oct 2024 15:00
Operator : SY/MD
Sample : P4379-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

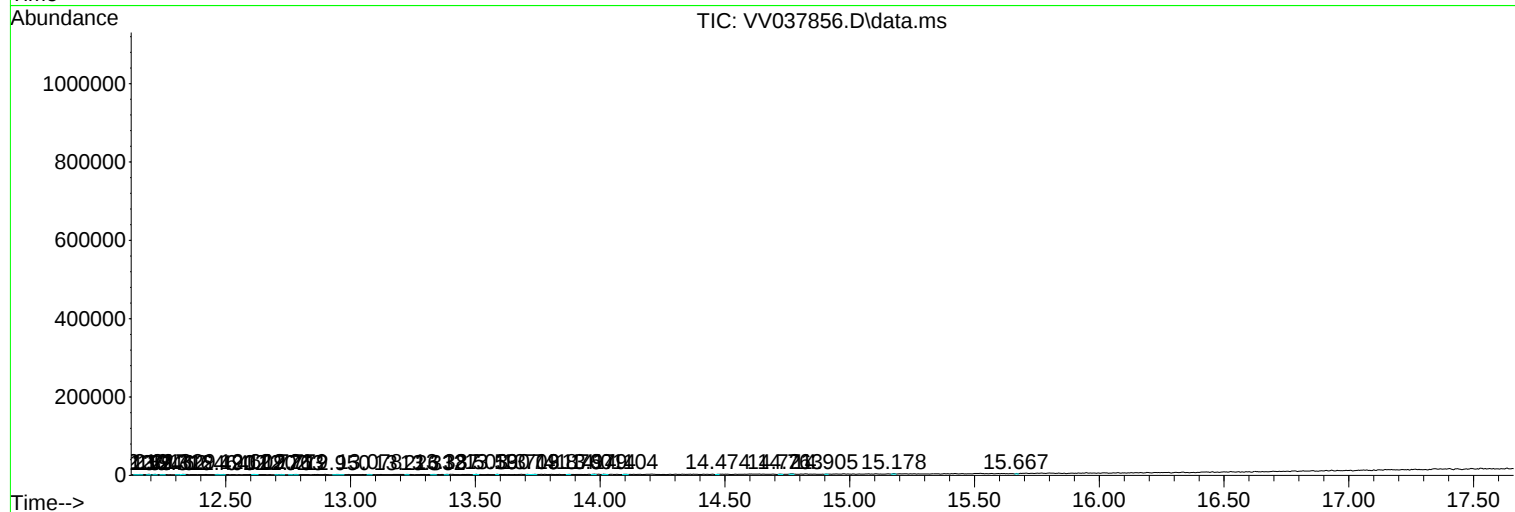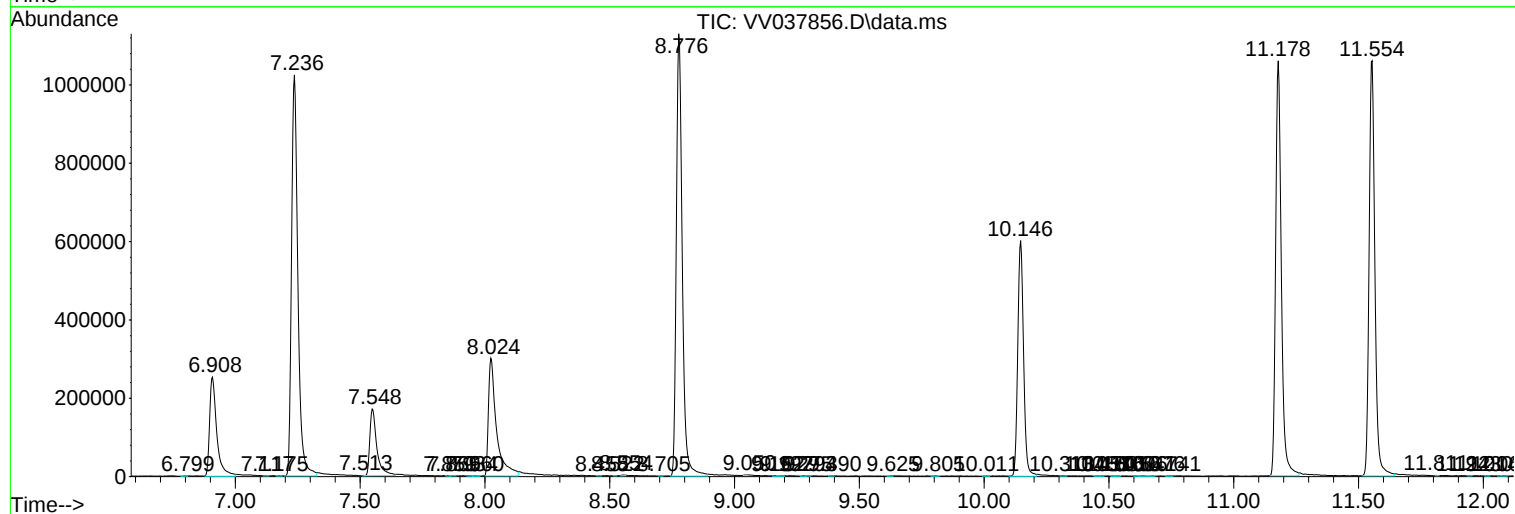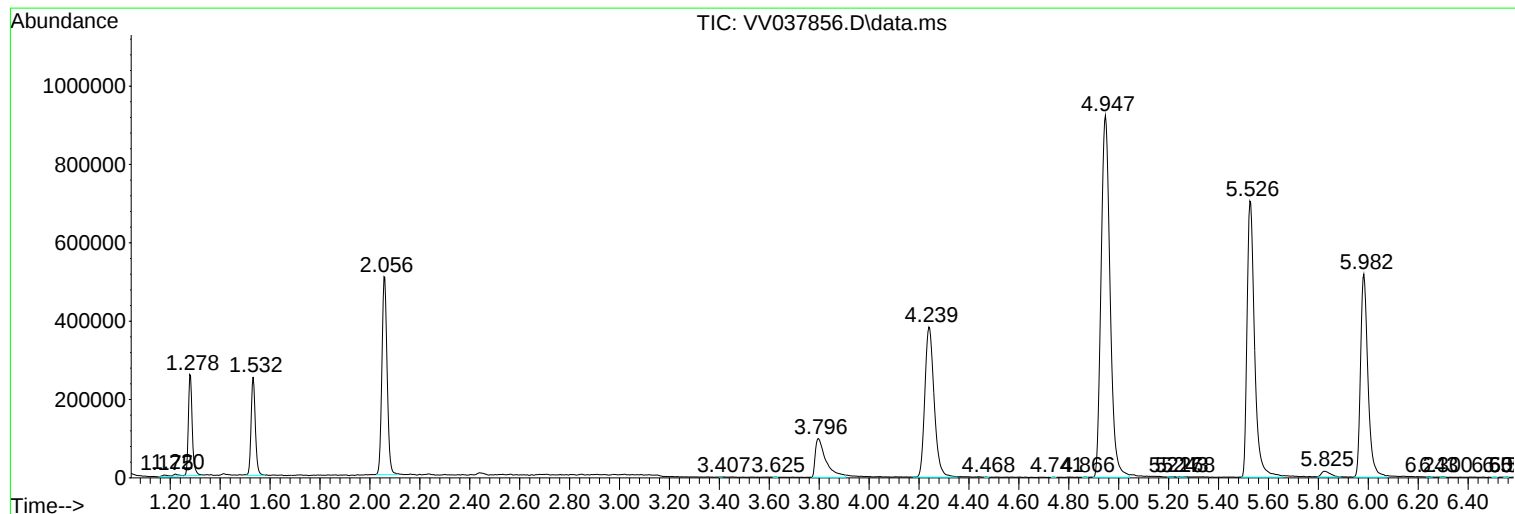

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037856.D
Acq On : 14 Oct 2024 15:00
Operator : SY/MD
Sample : P4379-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037856.D
Acq On : 14 Oct 2024 15:00
Operator : SY/MD
Sample : P4379-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------